
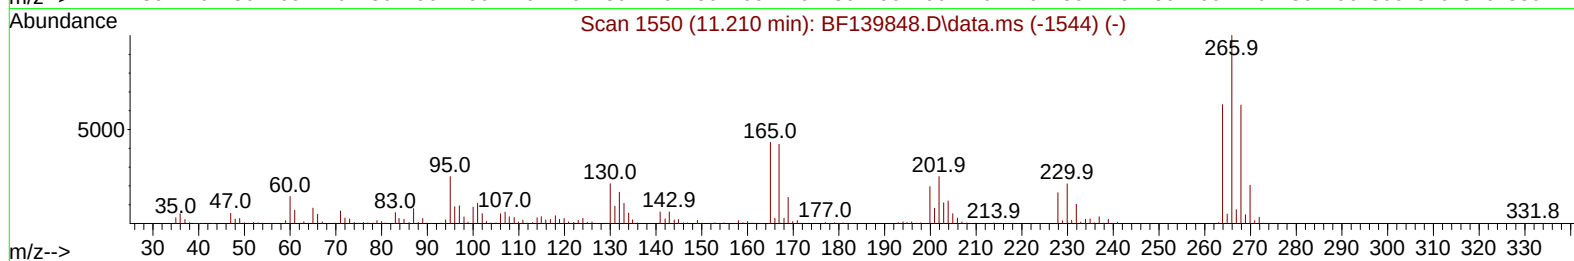
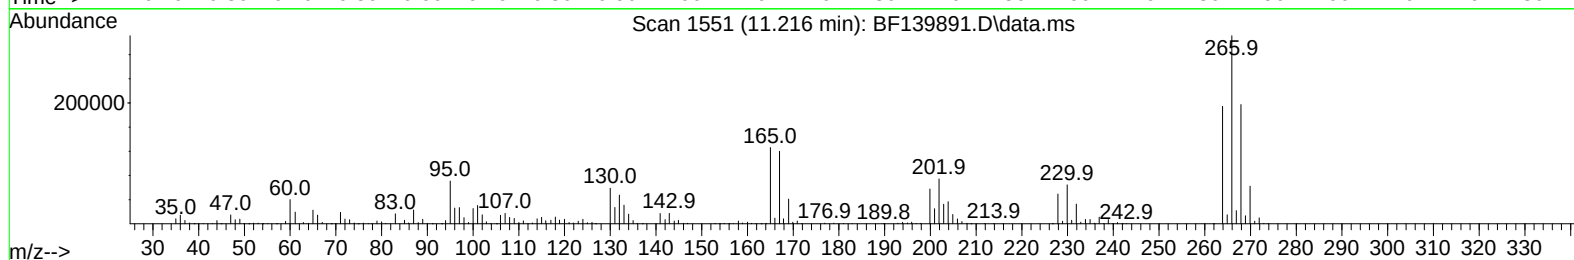


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF102124\
Data File : BF139891.D
Acq On : 21 Oct 2024 09:28
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 21 11:06:09 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF101824.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Oct 18 15:07:50 2024
Response via : Initial Calibration

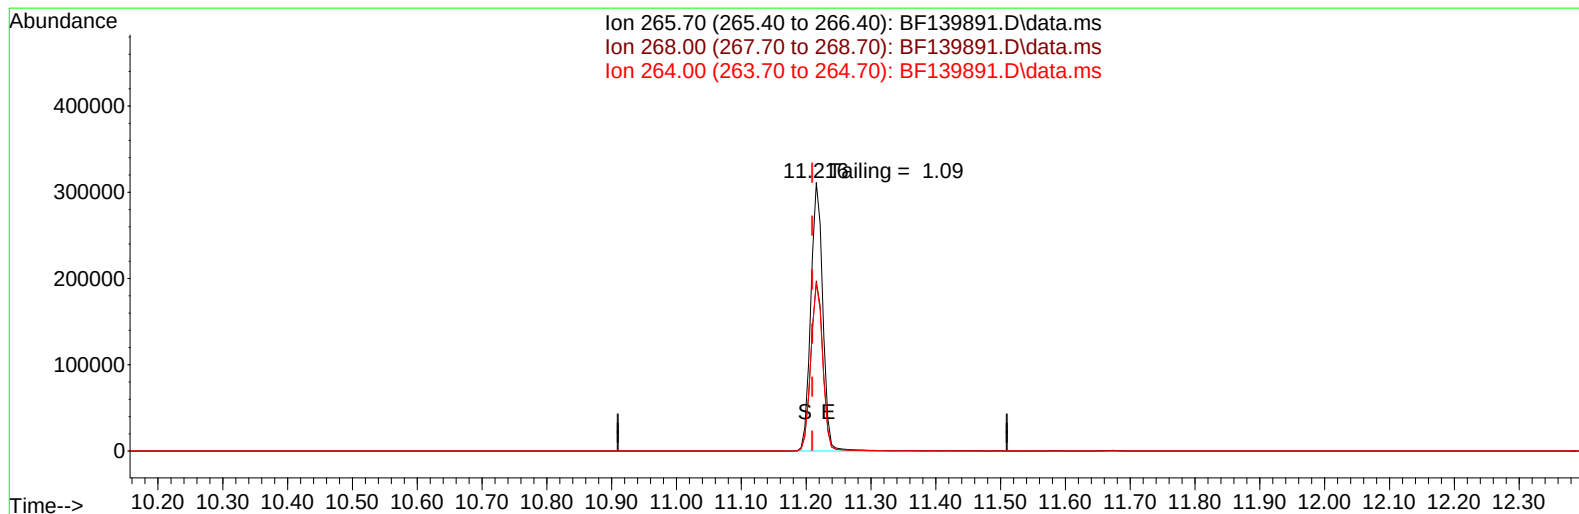

TIC: BF139891.D\data.ms

(70) Pentachlorophenol (C)




11.216min (+ 0.006) 62101.95 ng

response 401749

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.00	63.39
264.00	63.20	62.51
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF102124\
Data File : BF139891.D
Acq On : 21 Oct 2024 09:28
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 21 11:06:09 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF101824.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Oct 18 15:07:50 2024
Response via : Initial Calibration

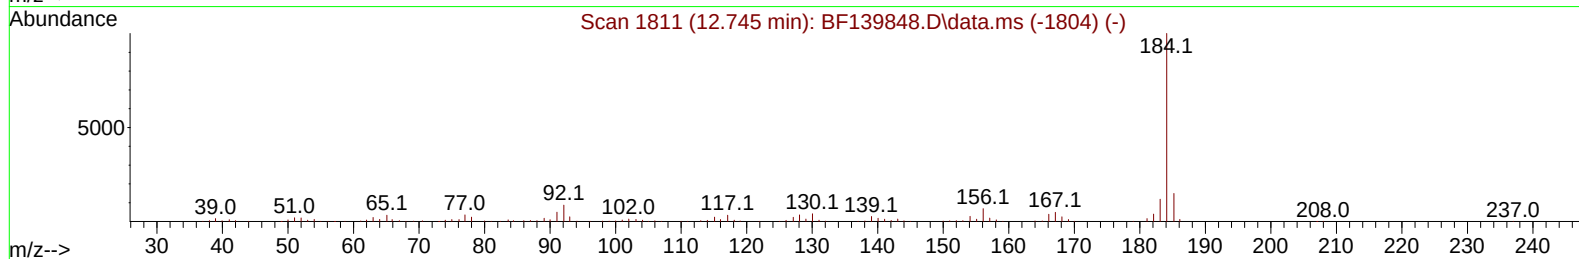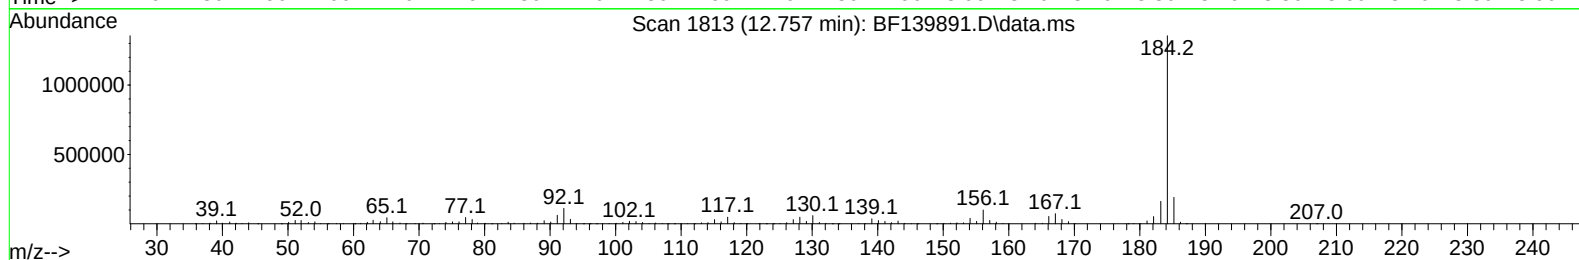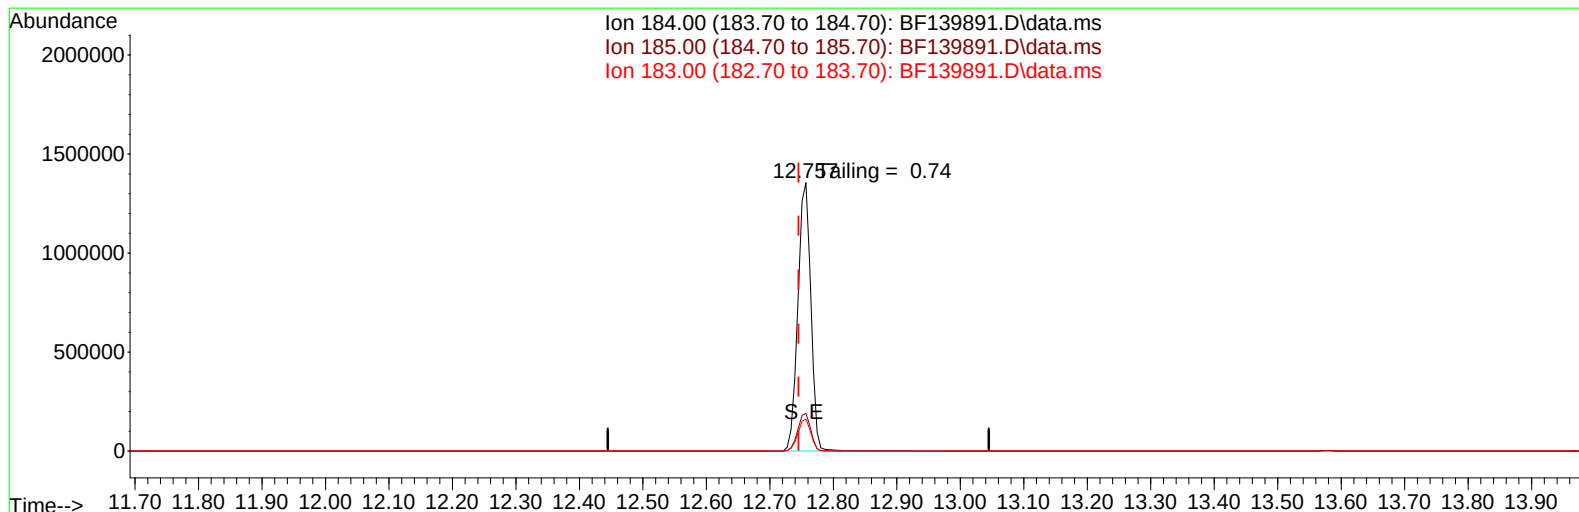

TIC: BF139891.D\data.ms

(77) Benzidine

12.757min (+ 0.012) 76266.80 ng

response 1925021

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.00	14.03
183.00	11.80	11.90
0.00	0.00	0.00