

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF102124\
 Data File : BF139908.D
 Acq On : 21 Oct 2024 17:39
 Operator : RC/JU
 Sample : P4395-01RE
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 F05308-SOLIDRE

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF101824.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF139908.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.187	8	16	27	rVB	1952012	3159161	93.04%	6.833%
2	3.993	312	323	337	rBV	43779	75102	2.21%	0.162%
3	5.116	508	514	520	rVB	161012	253398	7.46%	0.548%
4	5.322	542	549	556	rBV	39593	66288	1.95%	0.143%
5	5.387	556	560	565	rVB	31408	40396	1.19%	0.087%
6	5.504	568	580	585	rBV	2520202	3395588	100.00%	7.344%
7	5.669	604	608	613	rBV3	39174	65508	1.93%	0.142%
8	5.751	619	622	629	rVB5	36957	68759	2.02%	0.149%
9	5.828	629	635	643	rVB3	46104	94476	2.78%	0.204%
10	5.916	643	650	655	rBV4	169823	313512	9.23%	0.678%
11	5.963	655	658	663	rBV3	65423	111516	3.28%	0.241%
12	6.057	669	674	677	rBV3	130355	166324	4.90%	0.360%
13	6.098	677	681	684	rBV	123216	160075	4.71%	0.346%
14	6.146	684	689	696	rVV5	240466	536838	15.81%	1.161%
15	6.198	696	698	701	rVV	109584	108919	3.21%	0.236%
16	6.234	701	704	707	rVV3	75464	112511	3.31%	0.243%
17	6.287	711	713	716	rVB2	77922	79989	2.36%	0.173%
18	6.334	716	721	725	rBV2	182212	325167	9.58%	0.703%
19	6.375	725	728	733	rVB5	67132	104048	3.06%	0.225%
20	6.434	733	738	745	rBV3	326241	771833	22.73%	1.669%
21	6.504	745	750	755	rBV	2302163	3302022	97.24%	7.142%
22	6.546	755	757	759	rVV	113373	134932	3.97%	0.292%
23	6.569	759	761	764	rVB2	185562	182434	5.37%	0.395%
24	6.645	769	774	777	rVV4	243234	475602	14.01%	1.029%
25	6.675	777	779	784	rVV4	242376	307660	9.06%	0.665%
26	6.728	784	788	790	rVV2	171466	291448	8.58%	0.630%
27	6.751	790	792	796	rVB2	201204	211896	6.24%	0.458%
28	6.816	796	803	806	rBV5	156413	341021	10.04%	0.738%
29	6.857	806	810	812	rVV5	256038	426802	12.57%	0.923%
30	6.893	812	816	822	rVV2	938437	1435867	42.29%	3.105%
31	6.951	822	826	829	rVV2	261558	403946	11.90%	0.874%
32	7.004	829	835	838	rVV3	276283	660995	19.47%	1.430%
33	7.040	838	841	844	rVV2	311161	461850	13.60%	0.999%
34	7.069	844	846	851	rVV2	182820	247875	7.30%	0.536%
35	7.122	852	855	857	rVV3	110418	145113	4.27%	0.314%
36	7.163	858	862	866	rVB4	250536	386099	11.37%	0.835%

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF102124\
 Data File : BF139908.D
 Acq On : 21 Oct 2024 17:39
 Operator : RC/JU
 Sample : P4395-01RE
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 F05308-SOLIDRE

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF101824.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

37	7.204	866	869	872	rBV4	88537	117035	3.45%	0.253%
38	7.287	879	883	886	rBV2	214467	296352	8.73%	0.641%
39	7.316	886	888	894	rVB3	177290	242998	7.16%	0.526%
40	7.369	894	897	900	rBV2	61089	73512	2.16%	0.159%
41	7.445	900	910	916	rBV	1430063	2483891	73.15%	5.372%
42	7.534	921	925	929	rVB3	284213	454392	13.38%	0.983%
43	7.587	929	934	937	rBV3	108631	188866	5.56%	0.408%
44	7.675	946	949	950	rBV	66067	79998	2.36%	0.173%
45	7.698	950	953	960	rVB3	344417	504238	14.85%	1.091%
46	7.769	961	965	970	rBV6	160508	290408	8.55%	0.628%
47	7.816	970	973	980	rVB6	203698	258475	7.61%	0.559%
48	7.992	999	1003	1008	rBV4	96175	170399	5.02%	0.369%
49	8.045	1009	1012	1015	rBV4	85951	128167	3.77%	0.277%
50	8.122	1022	1025	1027	rBV4	59417	80657	2.38%	0.174%
51	8.169	1028	1033	1040	rVV	947506	1519842	44.76%	3.287%
52	8.228	1040	1043	1046	rVV	220981	274564	8.09%	0.594%
53	8.263	1046	1049	1056	rVB7	106910	177562	5.23%	0.384%
54	8.322	1057	1059	1062	rBV2	51460	69357	2.04%	0.150%
55	8.463	1080	1083	1089	rVB5	125834	199326	5.87%	0.431%
56	8.516	1090	1092	1096	rVB5	70974	76938	2.27%	0.166%
57	8.592	1102	1105	1111	rBV	430625	746970	22.00%	1.616%
58	8.681	1117	1120	1122	rBV2	71306	84343	2.48%	0.182%
59	8.716	1123	1126	1130	rVV4	88048	136422	4.02%	0.295%
60	8.922	1158	1161	1163	rBV2	86740	91007	2.68%	0.197%
61	8.957	1164	1167	1174	rVB6	86889	183044	5.39%	0.396%
62	9.051	1180	1183	1185	rBV4	94084	126146	3.71%	0.273%
63	9.192	1204	1207	1211	rVB	383950	455996	13.43%	0.986%
64	9.245	1211	1216	1221	rVB	2190482	2711153	79.84%	5.864%
65	9.328	1227	1230	1234	rBV3	193689	292422	8.61%	0.632%
66	9.586	1271	1274	1279	rVB	143482	186001	5.48%	0.402%
67	9.645	1279	1284	1290	rVB2	536755	779913	22.97%	1.687%
68	9.792	1306	1309	1313	rBV4	122339	177460	5.23%	0.384%
69	9.839	1314	1317	1321	rVB2	210935	263400	7.76%	0.570%
70	9.928	1327	1332	1336	rVB	847317	1090855	32.13%	2.359%
71	10.034	1347	1350	1354	rVB2	124243	163405	4.81%	0.353%
72	10.122	1362	1365	1369	rVB3	146161	195561	5.76%	0.423%
73	10.169	1370	1373	1382	rVB4	121471	280212	8.25%	0.606%
74	10.245	1382	1386	1388	rBV	123648	161045	4.74%	0.348%
75	10.333	1398	1401	1407	rVB5	122620	226627	6.67%	0.490%
76	10.639	1448	1453	1457	rVB	506108	665196	19.59%	1.439%

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF102124\
 Data File : BF139908.D
 Acq On : 21 Oct 2024 17:39
 Operator : RC/JU
 Sample : P4395-01RE
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 F05308-SOLIDRE

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF101824.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

77	10.710	1460	1465	1470	rVV	1189244	1536018	45.24%	3.322%
78	10.839	1484	1487	1494	rVB2	209812	299451	8.82%	0.648%
79	10.916	1496	1500	1502	rBV	70517	95641	2.82%	0.207%
80	10.945	1503	1505	1509	rVB2	83717	102913	3.03%	0.223%
81	11.016	1514	1517	1521	rVV	182746	283615	8.35%	0.613%
82	11.051	1521	1523	1535	rVB6	123433	290192	8.55%	0.628%
83	11.310	1563	1567	1573	rVB2	148416	237359	6.99%	0.513%
84	11.410	1580	1584	1592	rBV	781837	1116324	32.88%	2.414%
85	11.528	1600	1604	1610	rBV4	77681	162618	4.79%	0.352%
86	11.745	1638	1641	1651	rVB3	83940	164039	4.83%	0.355%
87	11.939	1667	1674	1678	rBV4	284678	477406	14.06%	1.033%
88	12.392	1748	1751	1758	rVB3	80075	153106	4.51%	0.331%
89	12.463	1760	1763	1766	rBV	134301	169790	5.00%	0.367%
90	12.627	1787	1791	1795	rBV	204310	256673	7.56%	0.555%
91	12.722	1804	1807	1814	rBV3	79342	128387	3.78%	0.278%
92	12.857	1826	1830	1836	rVV2	194348	341485	10.06%	0.739%
93	12.910	1837	1839	1843	rVB	93499	112385	3.31%	0.243%
94	12.998	1849	1854	1862	rVB	1813630	2368275	69.75%	5.122%
95	14.051	2028	2033	2041	rBV2	678199	1073424	31.61%	2.322%
96	15.533	2281	2285	2297	rVB	440706	738167	21.74%	1.597%


Sum of corrected areas: 46236393

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF102124\
Data File : BF139908.D
Acq On : 21 Oct 2024 17:39
Operator : RC/JU
Sample : P4395-01RE
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
F05308-SOLIDRE

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF101824.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

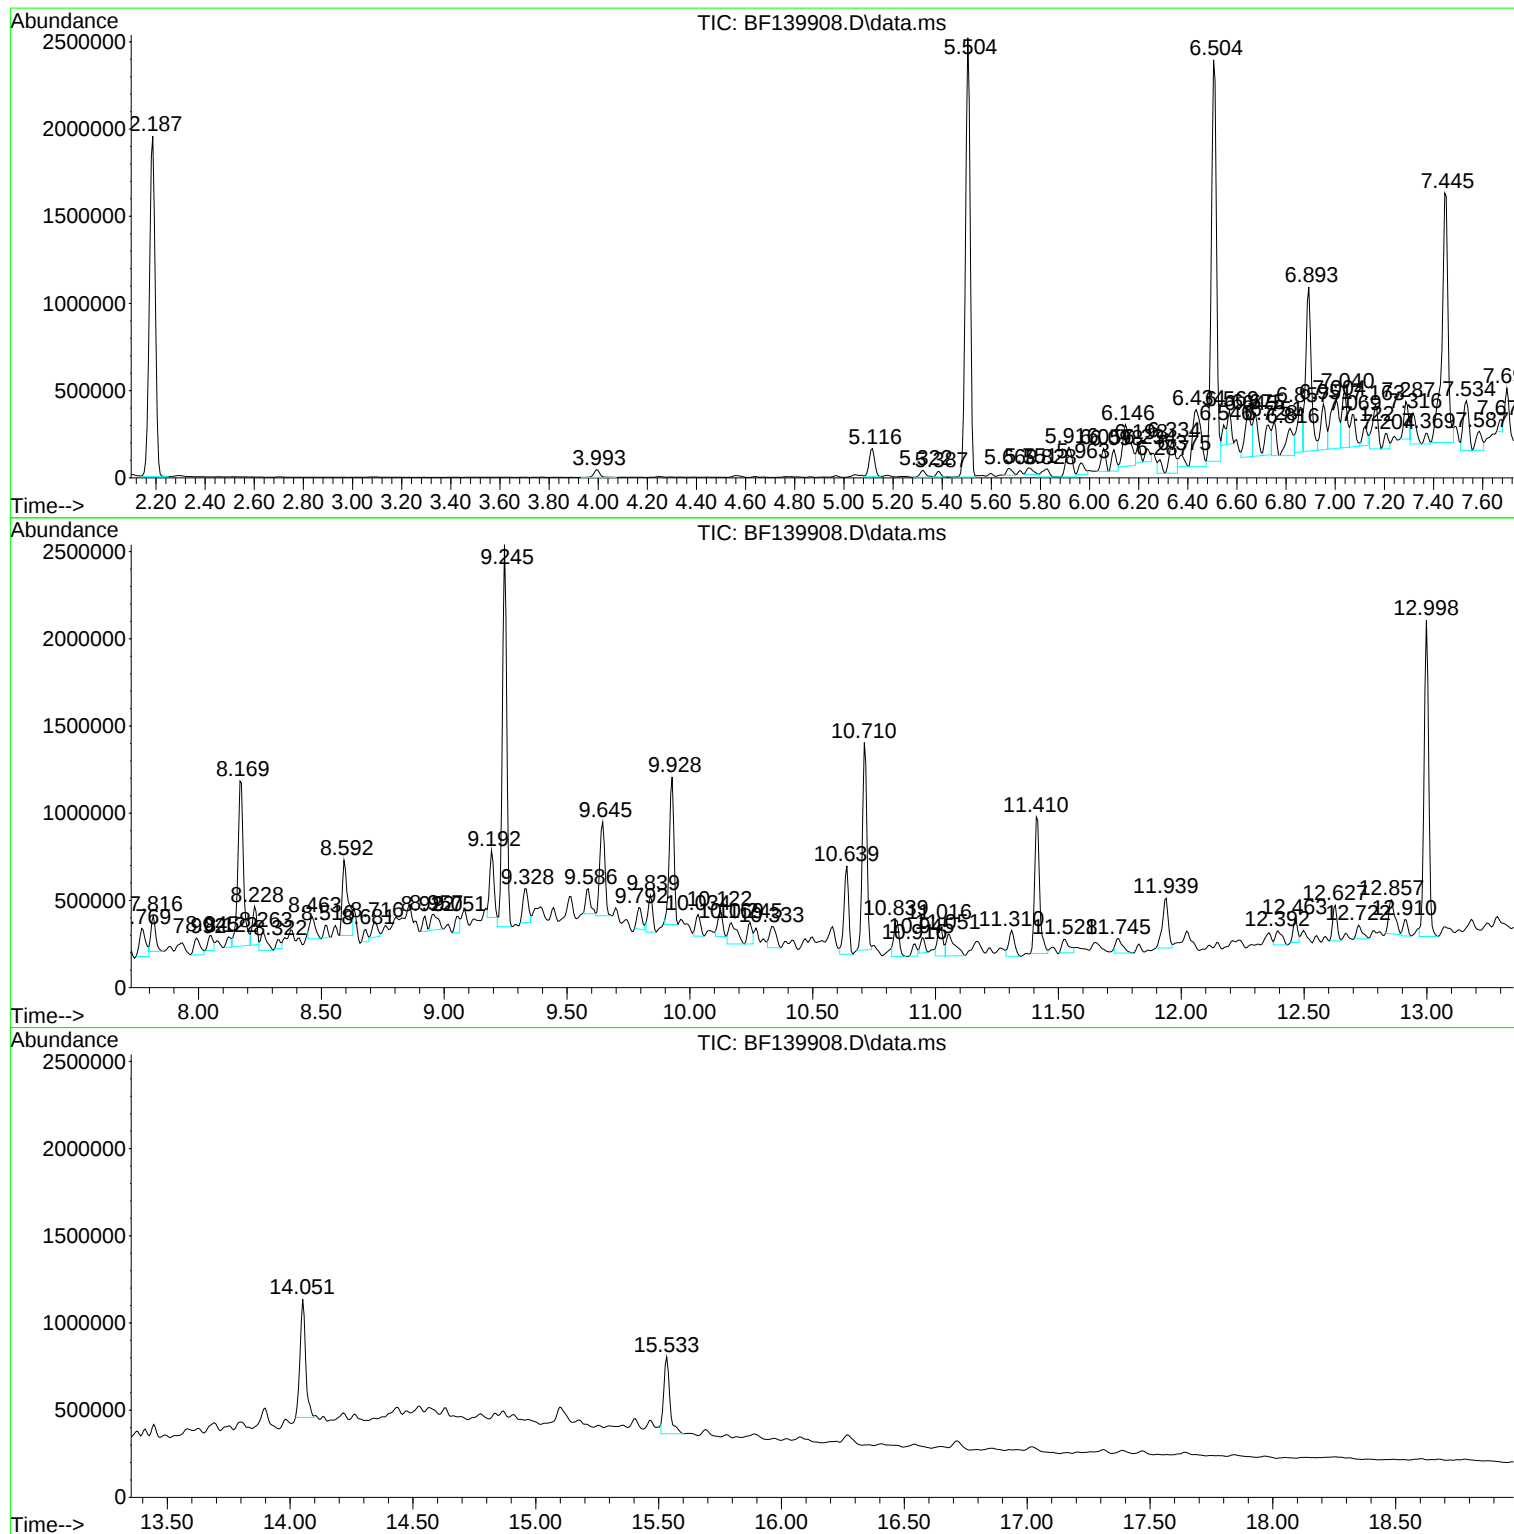

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF102124\
Data File : BF139908.D
Acq On : 21 Oct 2024 17:39
Operator : RC/JU
Sample : P4395-01RE
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
F05308-SOLIDRE

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF101824.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF102124\
Data File : BF139908.D
Acq On : 21 Oct 2024 17:39
Operator : RC/JU
Sample : P4395-01RE
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
F05308-SOLIDRE

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF101824.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------