

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF102124\
 Data File : BF139909.D
 Acq On : 21 Oct 2024 18:08
 Operator : RC/JU
 Sample : P4400-01RE 3X
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 NB-08-101424RE

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF101824.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF139909.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.152	3	10	18	rVB	551523	880540	75.77%	6.007%
2	3.975	314	320	328	rBV	10505	17624	1.52%	0.120%
3	5.093	504	510	519	rVB	30057	42725	3.68%	0.291%
4	5.492	573	578	587	rBV	507601	642285	55.27%	4.382%
5	6.498	744	749	760	rBV	500767	648096	55.77%	4.421%
6	6.892	811	816	821	rBV	684236	857130	73.75%	5.847%
7	7.163	852	862	866	rBV3	12216	22143	1.91%	0.151%
8	7.204	866	869	873	rBV	12028	17054	1.47%	0.116%
9	7.286	877	883	887	rBV3	14215	23396	2.01%	0.160%
10	7.375	892	898	902	rVB4	6714	12986	1.12%	0.089%
11	7.445	902	910	914	rBV	293323	393203	33.83%	2.682%
12	7.486	914	917	920	rVB	17353	21210	1.83%	0.145%
13	7.534	920	925	929	rVB4	19990	31248	2.69%	0.213%
14	7.575	929	932	935	rBV4	8253	12732	1.10%	0.087%
15	7.645	940	944	948	rBV2	22320	31540	2.71%	0.215%
16	7.698	948	953	961	rVB2	39072	65005	5.59%	0.443%
17	7.792	962	969	970	rBV2	14558	28178	2.42%	0.192%
18	7.816	970	973	977	rBV3	14352	16827	1.45%	0.115%
19	7.910	983	989	992	rBV4	24533	46266	3.98%	0.316%
20	8.010	1004	1006	1009	rVB	17314	17447	1.50%	0.119%
21	8.075	1014	1017	1021	rBV2	12863	16081	1.38%	0.110%
22	8.169	1021	1033	1040	rBV	799727	1162141	100.00%	7.928%
23	8.228	1040	1043	1046	rVB3	32482	44137	3.80%	0.301%
24	8.263	1046	1049	1055	rVB5	14434	21081	1.81%	0.144%
25	8.369	1057	1067	1072	rBV5	35241	77422	6.66%	0.528%
26	8.416	1072	1075	1078	rBV3	14074	17813	1.53%	0.122%
27	8.463	1078	1083	1087	rBV5	38250	58983	5.08%	0.402%
28	8.522	1090	1093	1095	rBV4	16500	16878	1.45%	0.115%
29	8.551	1095	1098	1102	rBV3	26760	31256	2.69%	0.213%
30	8.592	1102	1105	1107	rBV	27293	33119	2.85%	0.226%
31	8.675	1115	1119	1124	rBV4	68471	91489	7.87%	0.624%
32	8.763	1130	1134	1138	rBV	113318	145165	12.49%	0.990%
33	8.833	1143	1146	1148	rVB	18448	24054	2.07%	0.164%
34	8.922	1158	1161	1163	rBV2	17442	20196	1.74%	0.138%
35	8.992	1169	1173	1178	rBV3	65357	95061	8.18%	0.649%
36	9.122	1192	1195	1200	rVB3	39614	66055	5.68%	0.451%

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF102124\
 Data File : BF139909.D
 Acq On : 21 Oct 2024 18:08
 Operator : RC/JU
 Sample : P4400-01RE 3X
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 NB-08-101424RE

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF101824.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

37	9.169	1200	1203	1204	rBV2	19500	21567	1.86%	0.147%
38	9.192	1204	1207	1212	rVV3	56189	78067	6.72%	0.533%
39	9.245	1212	1216	1221	rVB	497132	594980	51.20%	4.059%
40	9.328	1225	1230	1234	rBV	218051	279586	24.06%	1.907%
41	9.398	1239	1242	1245	rVB	41986	49031	4.22%	0.334%
42	9.580	1267	1273	1275	rBV4	48989	98589	8.48%	0.673%
43	9.645	1280	1284	1287	rVV3	128104	206899	17.80%	1.411%
44	9.704	1291	1294	1298	rVB2	50458	64414	5.54%	0.439%
45	9.857	1315	1320	1324	rVB	261227	322697	27.77%	2.201%
46	9.928	1325	1332	1336	rBV	756864	960090	82.61%	6.550%
47	10.033	1347	1350	1354	rVB2	23413	27718	2.39%	0.189%
48	10.092	1356	1360	1362	rBV2	37456	61346	5.28%	0.419%
49	10.180	1371	1375	1379	rBV4	55059	76305	6.57%	0.521%
50	10.357	1400	1405	1409	rBV	308608	386704	33.28%	2.638%
51	10.575	1437	1442	1448	rBV	121571	201987	17.38%	1.378%
52	10.633	1449	1452	1455	rBV2	45997	53128	4.57%	0.362%
53	10.710	1460	1465	1469	rVB2	243209	323322	27.82%	2.206%
54	10.833	1481	1486	1495	rVB	368029	608657	52.37%	4.152%
55	11.280	1557	1562	1565	rBV	276821	366065	31.50%	2.497%
56	11.310	1565	1567	1573	rVB	118161	137163	11.80%	0.936%
57	11.416	1580	1585	1590	rBV	717355	950192	81.76%	6.482%
58	11.704	1630	1634	1639	rBV	236048	279762	24.07%	1.909%
59	11.933	1670	1673	1677	rVB3	53125	64899	5.58%	0.443%
60	12.116	1699	1704	1708	rBV	197264	249408	21.46%	1.702%
61	12.504	1766	1770	1774	rVB	154667	194948	16.77%	1.330%
62	12.874	1827	1833	1837	rVB2	106737	160794	13.84%	1.097%
63	12.998	1849	1854	1863	rVB	480744	635395	54.67%	4.335%
64	13.233	1890	1894	1899	rBV	68801	91438	7.87%	0.624%
65	13.574	1949	1952	1956	rBV	45229	53463	4.60%	0.365%
66	14.051	2029	2033	2040	rBV	567880	722058	62.13%	4.926%
67	15.533	2280	2285	2296	rVB	359265	588861	50.67%	4.017%




Sum of corrected areas: 14658099

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF102124\
Data File : BF139909.D
Acq On : 21 Oct 2024 18:08
Operator : RC/JU
Sample : P4400-01RE 3X
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
NB-08-101424RE

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF101824.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

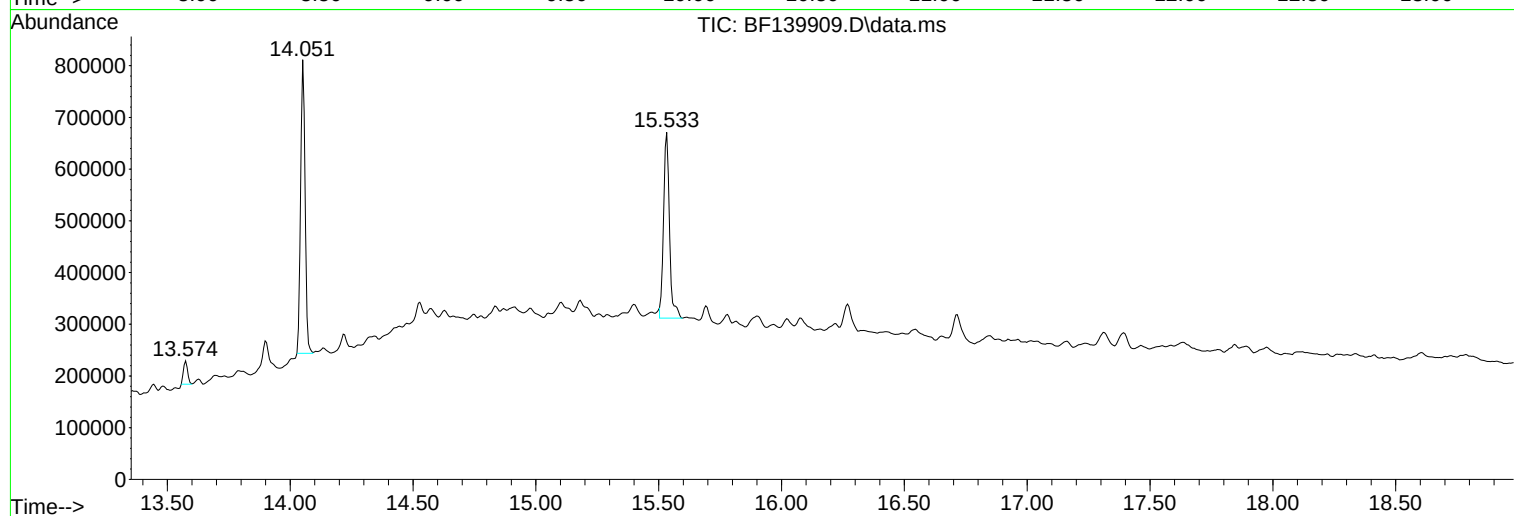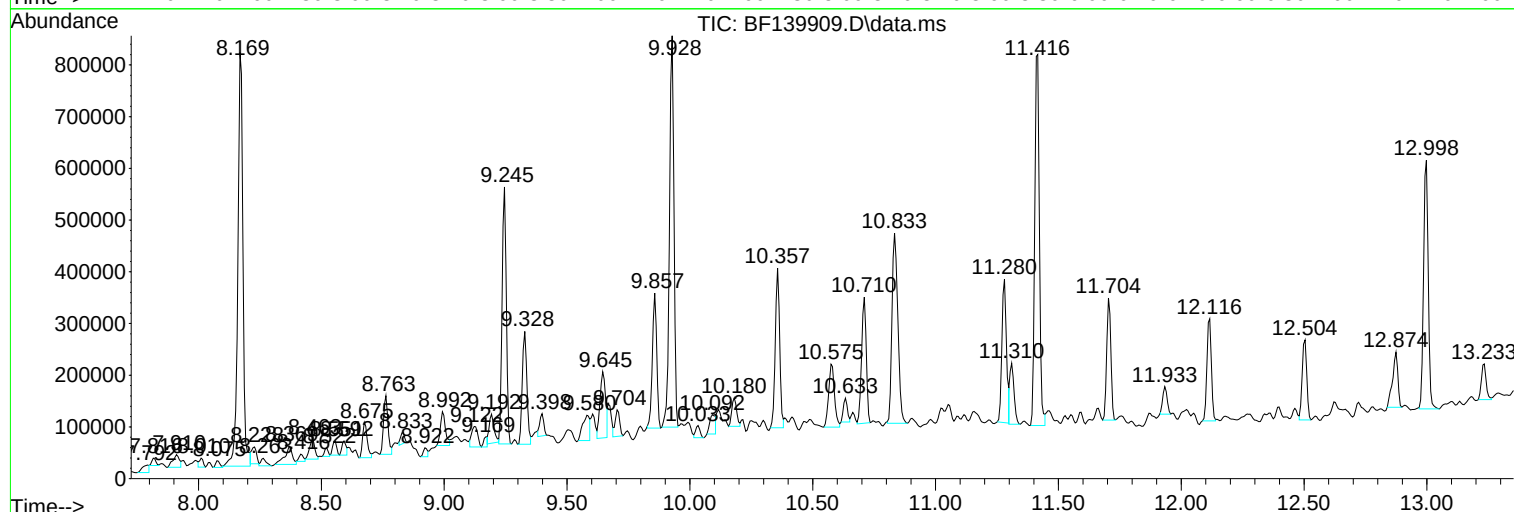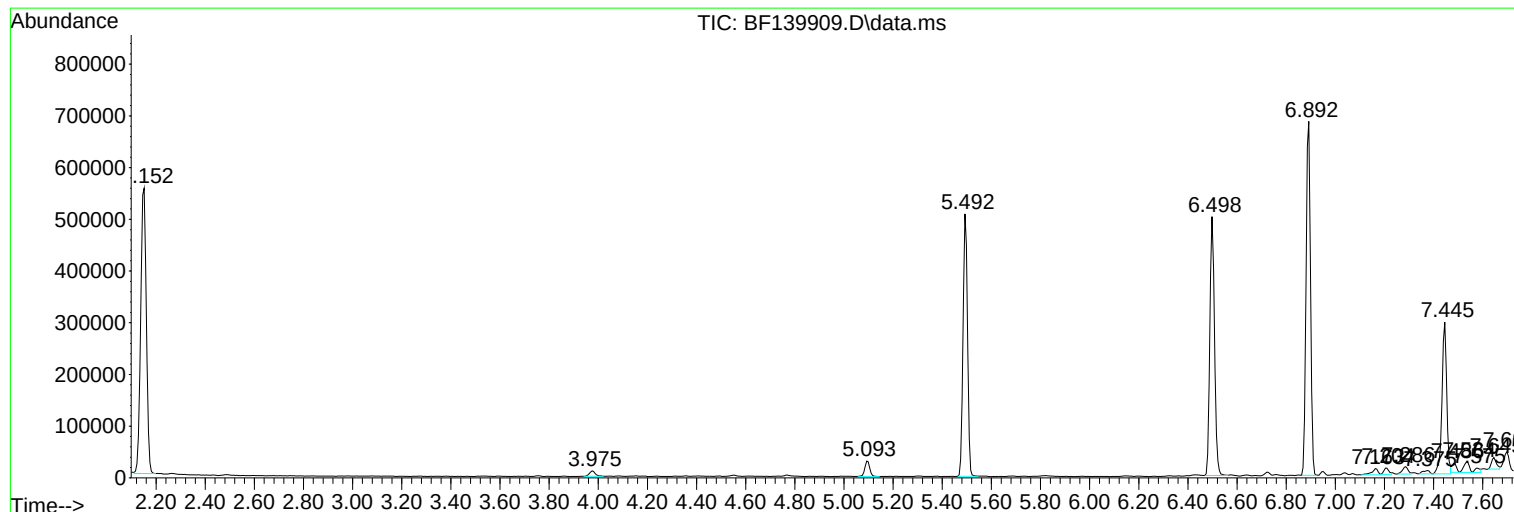

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF102124\
Data File : BF139909.D
Acq On : 21 Oct 2024 18:08
Operator : RC/JU
Sample : P4400-01RE 3X
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
NB-08-101424RE

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF101824.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF102124\
Data File : BF139909.D
Acq On : 21 Oct 2024 18:08
Operator : RC/JU
Sample : P4400-01RE 3X
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
NB-08-101424RE

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF101824.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------