

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF102124\
 Data File : BF139911.D
 Acq On : 21 Oct 2024 19:06
 Operator : RC/JU
 Sample : P4406-01RE 5X
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 OK-02-101524RE

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF101824.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF139911.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.152	3	10	17	rBV	493494	766820	48.00%	4.248%
2	3.975	315	320	327	rVB	10971	18167	1.14%	0.101%
3	5.099	506	511	518	rVB	32119	43419	2.72%	0.241%
4	5.498	573	579	590	rBV	505102	650965	40.74%	3.606%
5	6.498	744	749	760	rBV	493368	625160	39.13%	3.463%
6	6.893	811	816	821	rBV	747377	913387	57.17%	5.060%
7	7.445	902	910	915	rBV	283804	354451	22.19%	1.963%
8	7.516	915	922	929	rVB5	12093	26795	1.68%	0.148%
9	7.698	948	953	960	rVB3	16474	21303	1.33%	0.118%
10	7.916	982	990	995	rBV6	7670	19263	1.21%	0.107%
11	8.175	1028	1034	1041	rBV	803418	1080112	67.61%	5.983%
12	8.681	1116	1120	1130	rBV6	10700	25864	1.62%	0.143%
13	8.816	1137	1143	1151	rBV9	8893	25760	1.61%	0.143%
14	8.886	1151	1155	1159	rVB	38109	46201	2.89%	0.256%
15	8.986	1167	1172	1177	rBV	40437	54590	3.42%	0.302%
16	9.245	1211	1216	1221	rBV	497101	594861	37.23%	3.295%
17	9.328	1226	1230	1237	rBV2	17738	37407	2.34%	0.207%
18	9.445	1247	1250	1255	rVB2	13402	19390	1.21%	0.107%
19	9.510	1256	1261	1265	rBV	35195	55420	3.47%	0.307%
20	9.586	1269	1274	1276	rVV	47900	66863	4.19%	0.370%
21	9.610	1276	1278	1281	rVV	32512	34836	2.18%	0.193%
22	9.645	1281	1284	1290	rVB2	37999	50085	3.13%	0.277%
23	9.704	1290	1294	1303	rVB	32127	56268	3.52%	0.312%
24	9.786	1303	1308	1314	rBV	189954	246588	15.43%	1.366%
25	9.857	1317	1320	1324	rVB	13424	17422	1.09%	0.097%
26	9.928	1325	1332	1336	rBV	839288	1051508	65.81%	5.825%
27	9.957	1336	1337	1341	rVB	33803	31089	1.95%	0.172%
28	10.033	1346	1350	1354	rVV	13885	17802	1.11%	0.099%
29	10.128	1362	1366	1370	rVB	40749	52938	3.31%	0.293%
30	10.169	1370	1373	1381	rVB	27625	35890	2.25%	0.199%
31	10.239	1381	1385	1388	rBV2	39236	60473	3.79%	0.335%
32	10.333	1396	1401	1402	rBV2	22083	32577	2.04%	0.180%
33	10.381	1407	1409	1412	rVB	30607	29863	1.87%	0.165%
34	10.475	1421	1425	1431	rVB2	70365	112048	7.01%	0.621%
35	10.581	1440	1443	1447	rVB2	28252	36798	2.30%	0.204%
36	10.633	1448	1452	1460	rVB2	52590	93414	5.85%	0.517%

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF102124\
 Data File : BF139911.D
 Acq On : 21 Oct 2024 19:06
 Operator : RC/JU
 Sample : P4406-01RE 5X
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 OK-02-101524RE

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF101824.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

37	10.710	1460	1465	1470	rBV2	268675	346551	21.69%	1.920%
38	10.839	1482	1487	1492	rVB2	67439	104242	6.52%	0.577%
39	10.916	1497	1500	1503	rBV2	15257	20268	1.27%	0.112%
40	11.022	1514	1518	1520	rBV2	37379	52960	3.31%	0.293%
41	11.104	1530	1532	1536	rVB	18764	20040	1.25%	0.111%
42	11.216	1549	1551	1555	rVB2	27050	31983	2.00%	0.177%
43	11.310	1564	1567	1572	rVB	74523	98402	6.16%	0.545%
44	11.416	1580	1585	1587	rBV	820842	1108797	69.40%	6.142%
45	11.486	1593	1597	1600	rBV	104487	130445	8.16%	0.723%
46	11.710	1632	1635	1638	rVV2	40596	45213	2.83%	0.250%
47	11.745	1638	1641	1646	rVB	64051	76882	4.81%	0.426%
48	11.827	1653	1655	1659	rVB	48100	53421	3.34%	0.296%
49	11.869	1659	1662	1665	rBV3	26238	37164	2.33%	0.206%
50	11.916	1666	1670	1672	rBV	167554	227337	14.23%	1.259%
51	11.945	1672	1675	1679	rVB	210568	270963	16.96%	1.501%
52	11.992	1679	1683	1685	rBV	55399	72783	4.56%	0.403%
53	12.027	1685	1689	1691	rBV	205620	279264	17.48%	1.547%
54	12.116	1701	1704	1707	rVB	38833	41512	2.60%	0.230%
55	12.151	1707	1710	1713	rVB2	38270	43331	2.71%	0.240%
56	12.210	1717	1720	1722	rBV2	72542	91552	5.73%	0.507%
57	12.357	1740	1745	1748	rBV2	52959	100442	6.29%	0.556%
58	12.392	1748	1751	1753	rBV	58403	66412	4.16%	0.368%
59	12.463	1759	1763	1766	rBV	213990	304170	19.04%	1.685%
60	12.504	1766	1770	1775	rVV2	161127	298584	18.69%	1.654%
61	12.551	1775	1778	1782	rVV3	75391	104010	6.51%	0.576%
62	12.627	1787	1791	1795	rVB	568612	685866	42.93%	3.799%
63	12.674	1796	1799	1804	rBV4	47336	93863	5.87%	0.520%
64	12.722	1804	1807	1810	rVV2	56704	63259	3.96%	0.350%
65	12.857	1825	1830	1836	rBV	678664	1010280	63.23%	5.596%
66	12.916	1837	1840	1843	rVB3	84631	105170	6.58%	0.583%
67	12.998	1850	1854	1862	rVB	479876	694856	43.49%	3.849%
68	13.074	1863	1867	1874	rBV3	142892	286987	17.96%	1.590%
69	13.180	1879	1885	1889	rVB2	142801	317281	19.86%	1.758%
70	13.245	1891	1896	1900	rBV2	68783	150825	9.44%	0.835%
71	13.286	1900	1903	1908	rVV2	141432	182083	11.40%	1.009%
72	13.380	1916	1919	1922	rBV2	126407	142981	8.95%	0.792%
73	13.410	1922	1924	1928	rVB2	97831	102829	6.44%	0.570%
74	14.051	2028	2033	2045	rBV2	762712	1597678	100.00%	8.850%
75	15.104	2208	2212	2220	rVB	229197	496356	31.07%	2.749%
76	15.468	2271	2274	2280	rVB	180340	257223	16.10%	1.425%

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF102124\
Data File : BF139911.D
Acq On : 21 Oct 2024 19:06
Operator : RC/JU
Sample : P4406-01RE 5X
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
OK-02-101524RE

Integration Parameters: rteint.p
Integrator: RTE
Smoothing : ON Filtering: 5
Sampling : 1 Min Area: 3 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF101824.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

77	15.539	2282	2286	2290	rBV	293710	432631	27.08%	2.396%
----	--------	------	------	------	-----	--------	--------	--------	--------




Sum of corrected areas: 18052693

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF102124\
Data File : BF139911.D
Acq On : 21 Oct 2024 19:06
Operator : RC/JU
Sample : P4406-01RE 5X
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
OK-02-101524RE

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF101824.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

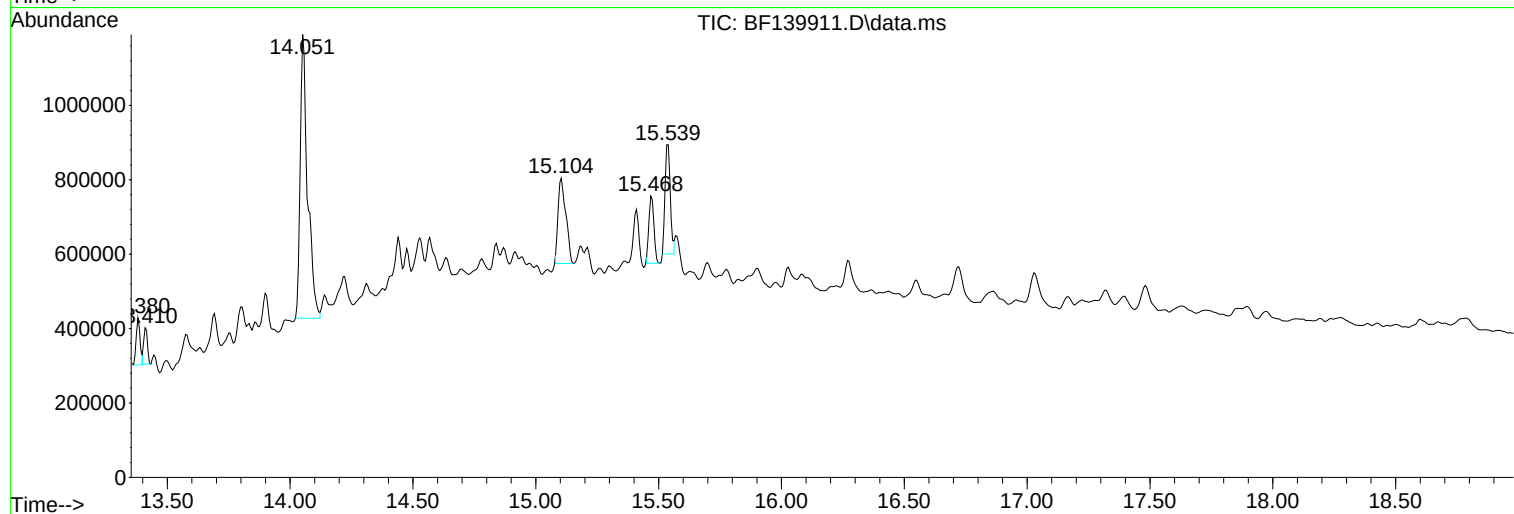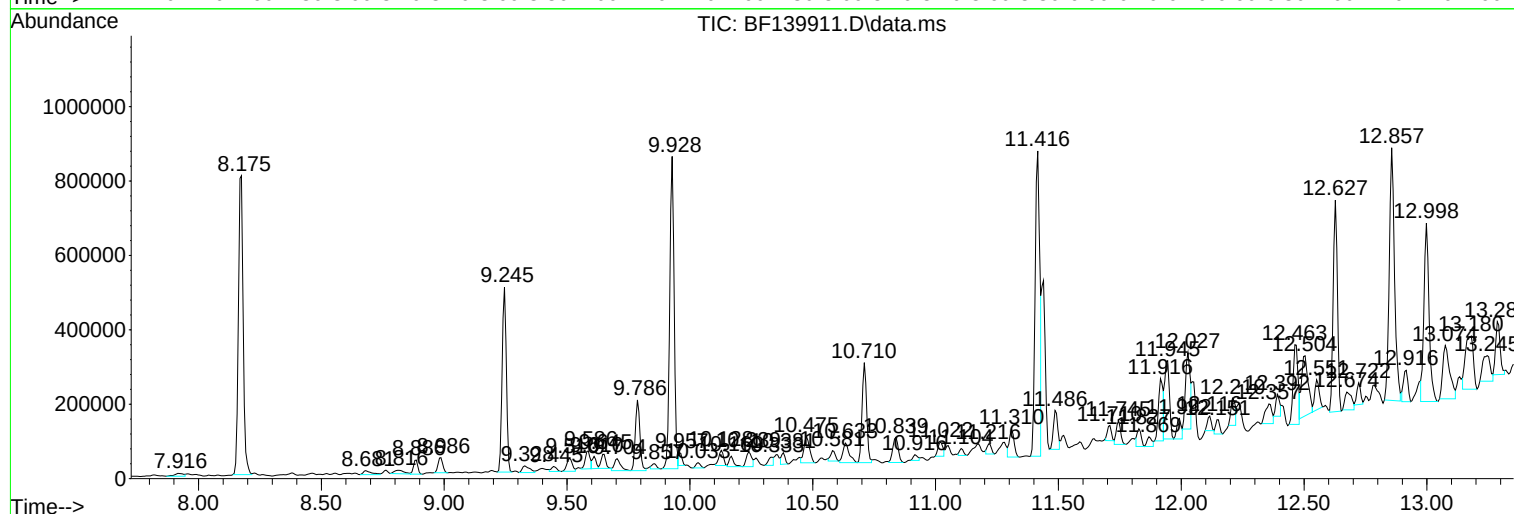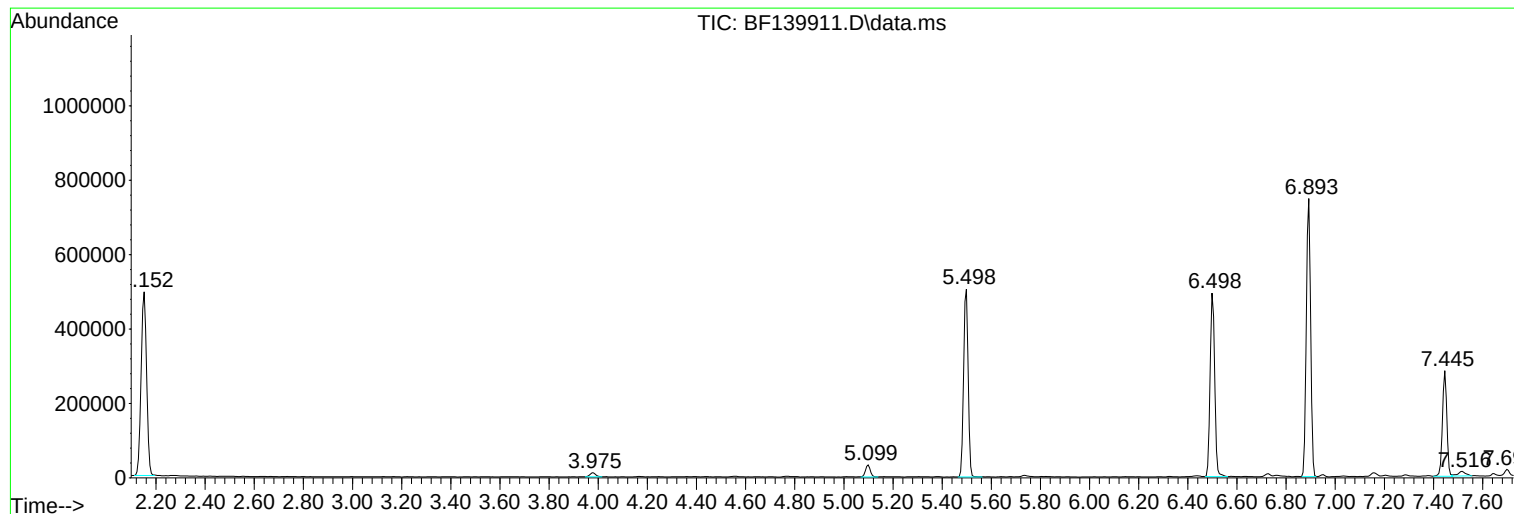

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF102124\
Data File : BF139911.D
Acq On : 21 Oct 2024 19:06
Operator : RC/JU
Sample : P4406-01RE 5X
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
OK-02-101524RE

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF101824.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF102124\
Data File : BF139911.D
Acq On : 21 Oct 2024 19:06
Operator : RC/JU
Sample : P4406-01RE 5X
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
OK-02-101524RE

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF101824.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------