
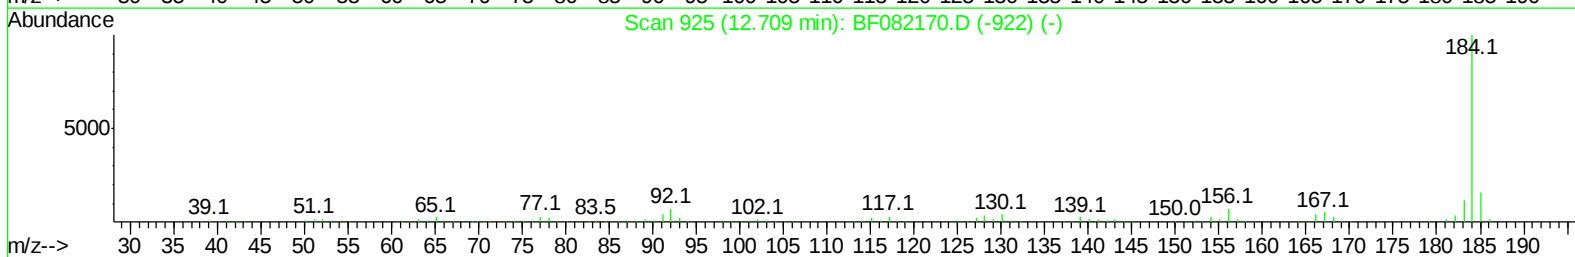
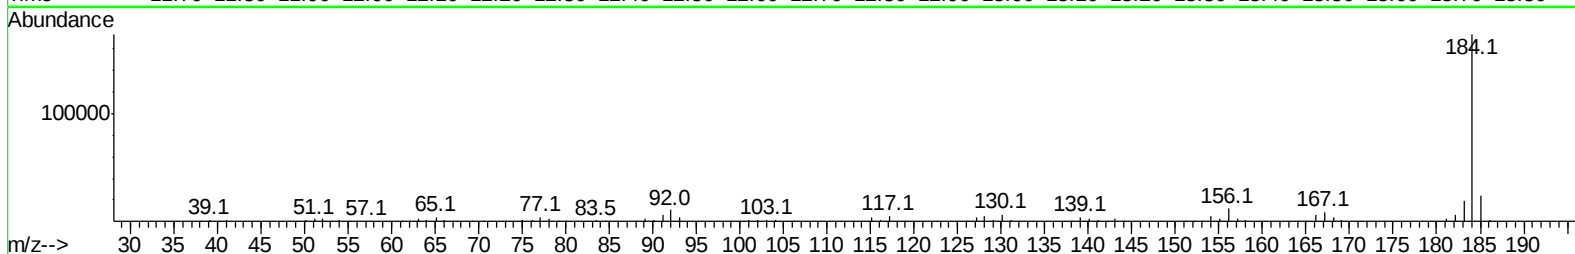


Data Path : Z:\HPCHEM1\BNA F\Data\bf102215\
Data File : BF082446.D
Acq On : 22 Oct 2015 14:33
Operator : UM/IZ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 23 05:04:40 2015
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF101015.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Oct 21 13:20:24 2015
Response via : Initial Calibration

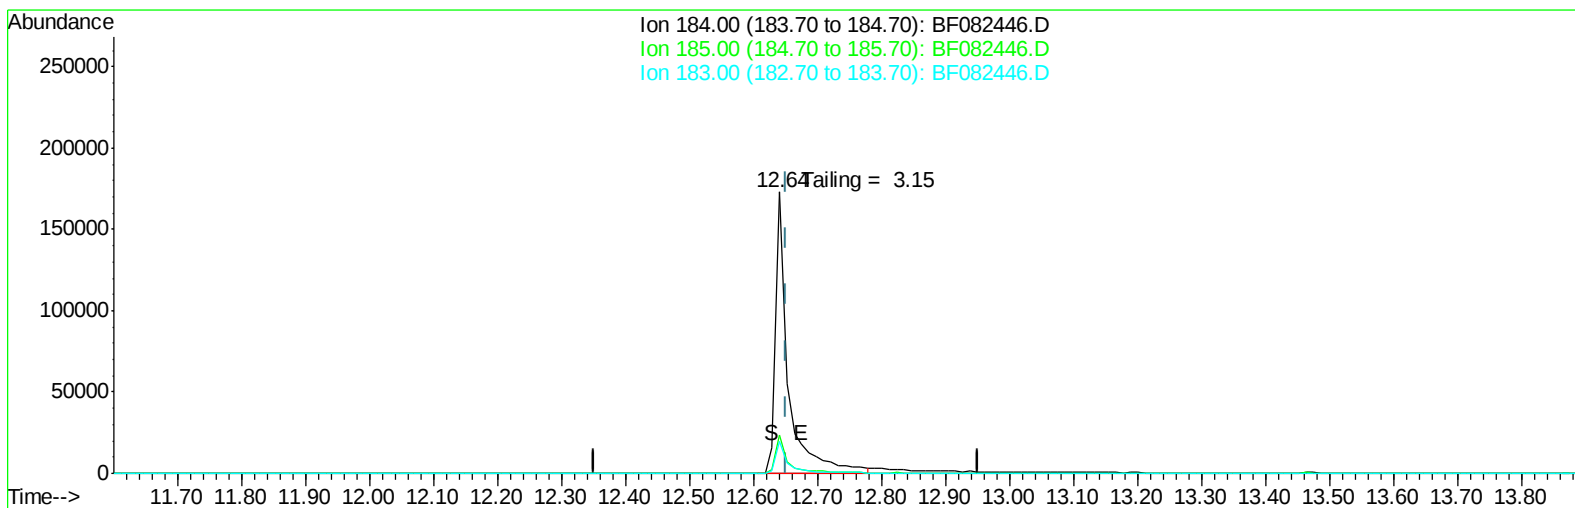

TIC: BF082446.D

(76) Benzidine




12.641min (-0.012) 0.00ng

response 250892

Ion	Exp%	Act%
184.00	100	100
185.00	15.60	13.86
183.00	11.40	11.34
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA F\Data\bf102215\
Data File : BF082446.D
Acq On : 22 Oct 2015 14:33
Operator : UM/IZ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 23 05:04:40 2015
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF101015.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Oct 21 13:20:24 2015
Response via : Initial Calibration

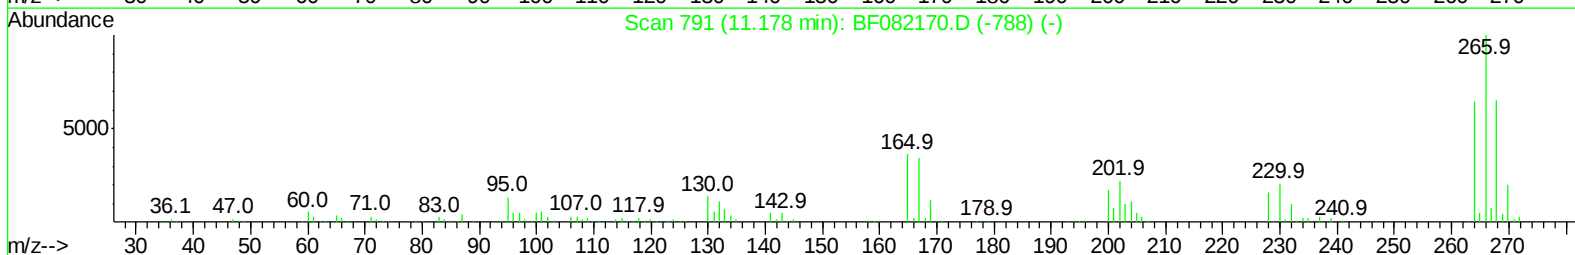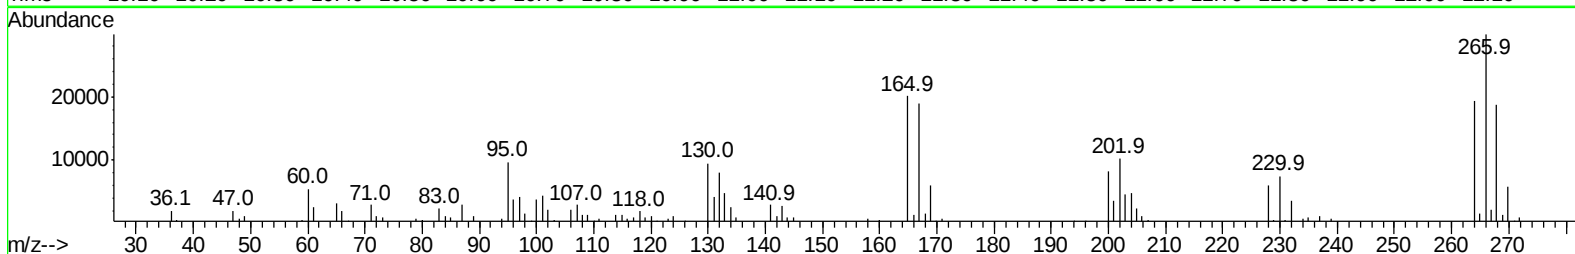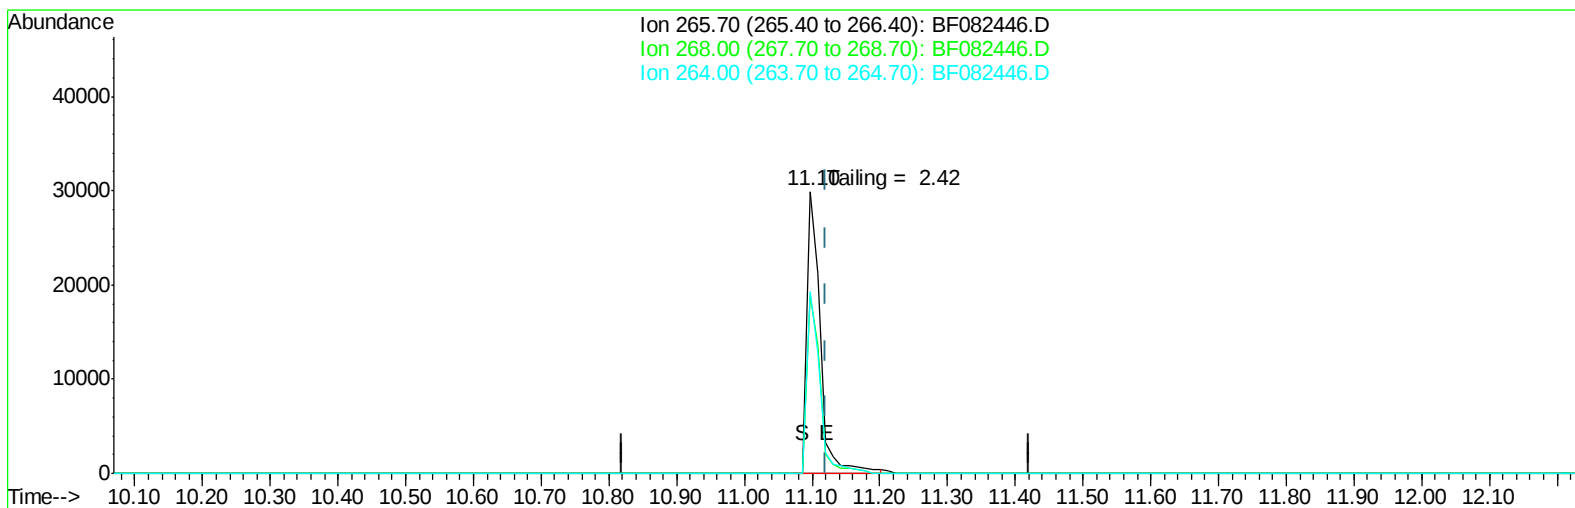

TIC: BF082446.D

(69) Pentachlorophenol (C)

11.098min (-0.023) 0.00ng

response 41225

Ion	Exp%	Act%
265.70	100	100
268.00	65.00	63.06
264.00	64.20	64.48
0.00	0.00	0.00