


Data Path : Z:\HPCHEM1\BNA_F\DATA\BF102215\
 Data File : BF082446.D
 Acq On : 22 Oct 2015 14:33
 Operator : UM/IZ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF101015.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Oct 23 15:17:13 2015

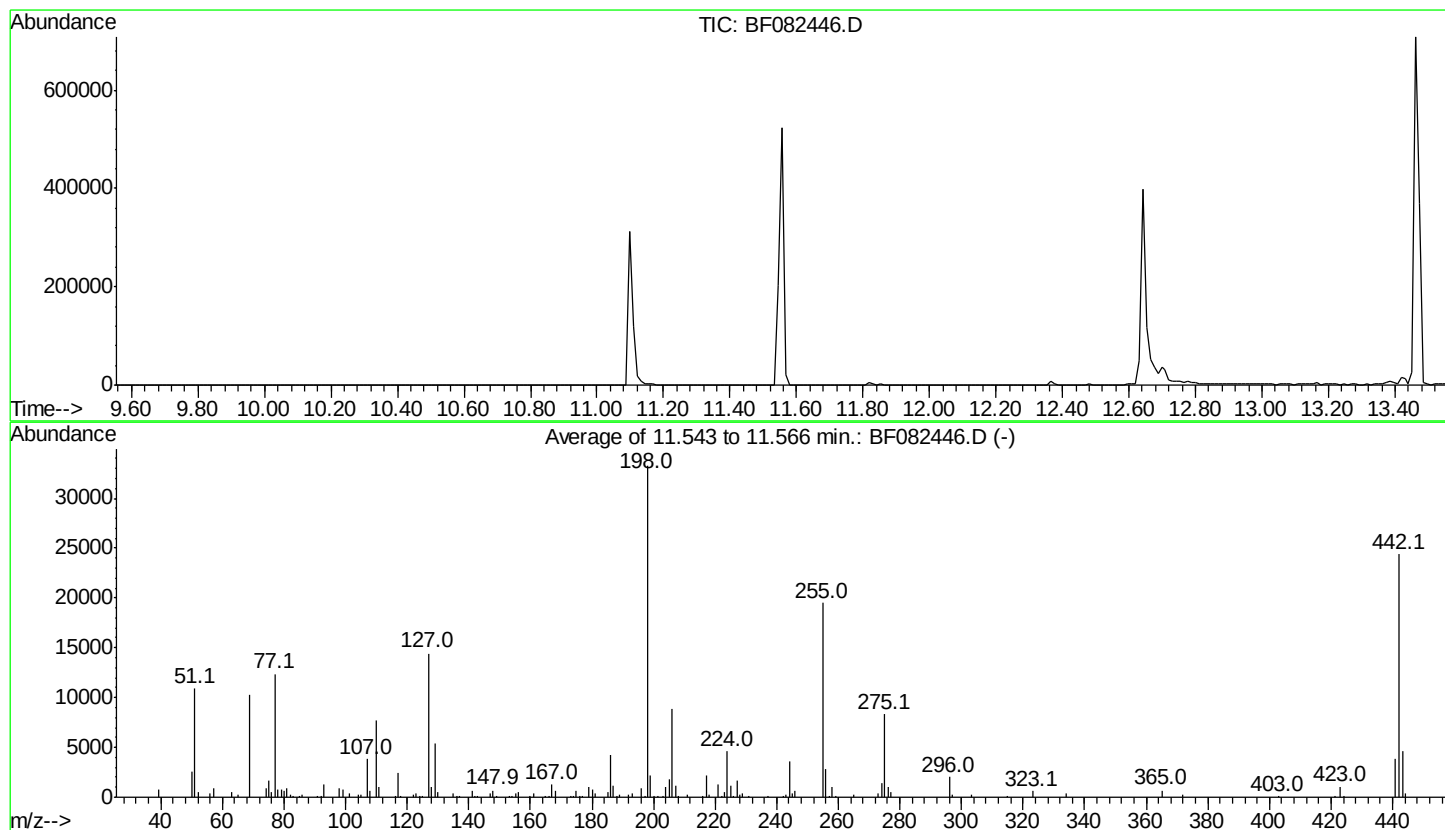

AutoFind: Scans 823, 824, 825; Background Corrected with Scan 820

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	32.7	10875	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	31.0	10316	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	43.2	14391	PASS
197	198	0.00	2	0.5	157	PASS
198	198	100	100	100.0	33281	PASS
199	198	5	9	6.7	2218	PASS
275	198	10	60	24.9	8300	PASS
365	198	1	100	2.0	653	PASS
441	442	0.01	24	15.7	3825	PASS
442	198	50	100	73.2	24365	PASS
443	442	15	24	19.1	4652	PASS