
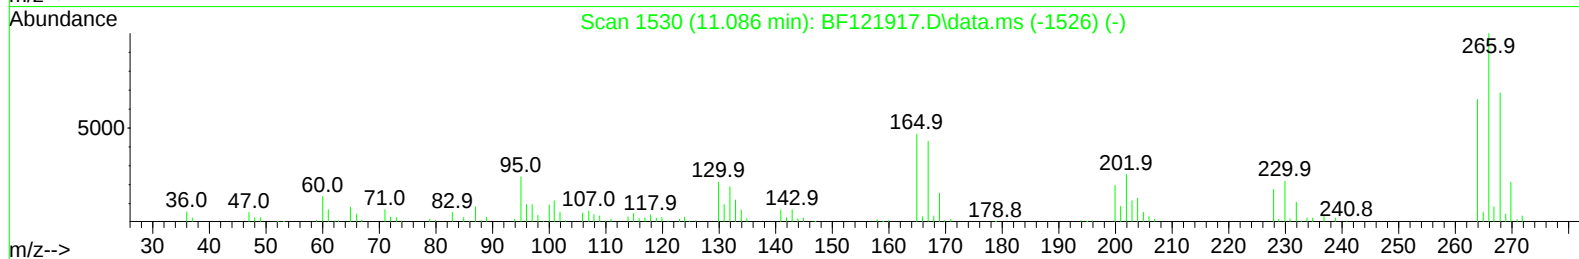
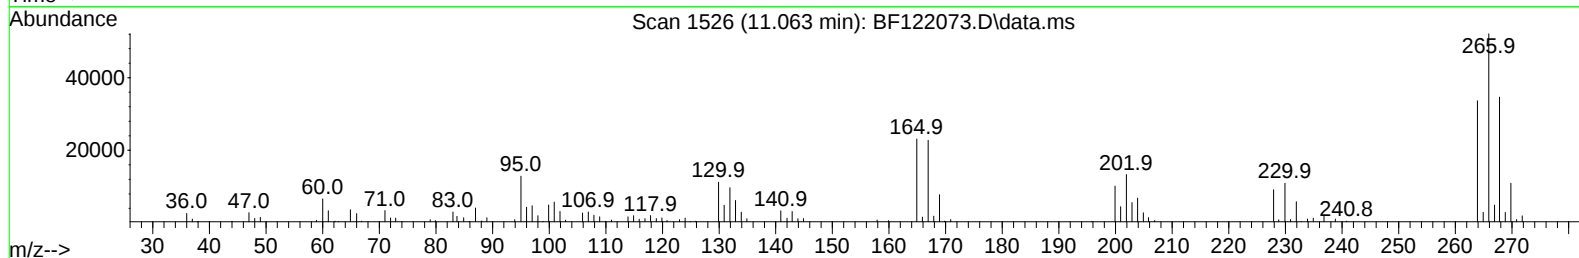


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF102220\
Data File : BF122073.D
Acq On : 22 Oct 2020 9:05
Operator : JU/CG
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 23 04:09:29 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF101220.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Oct 21 12:04:42 2020
Response via : Initial Calibration

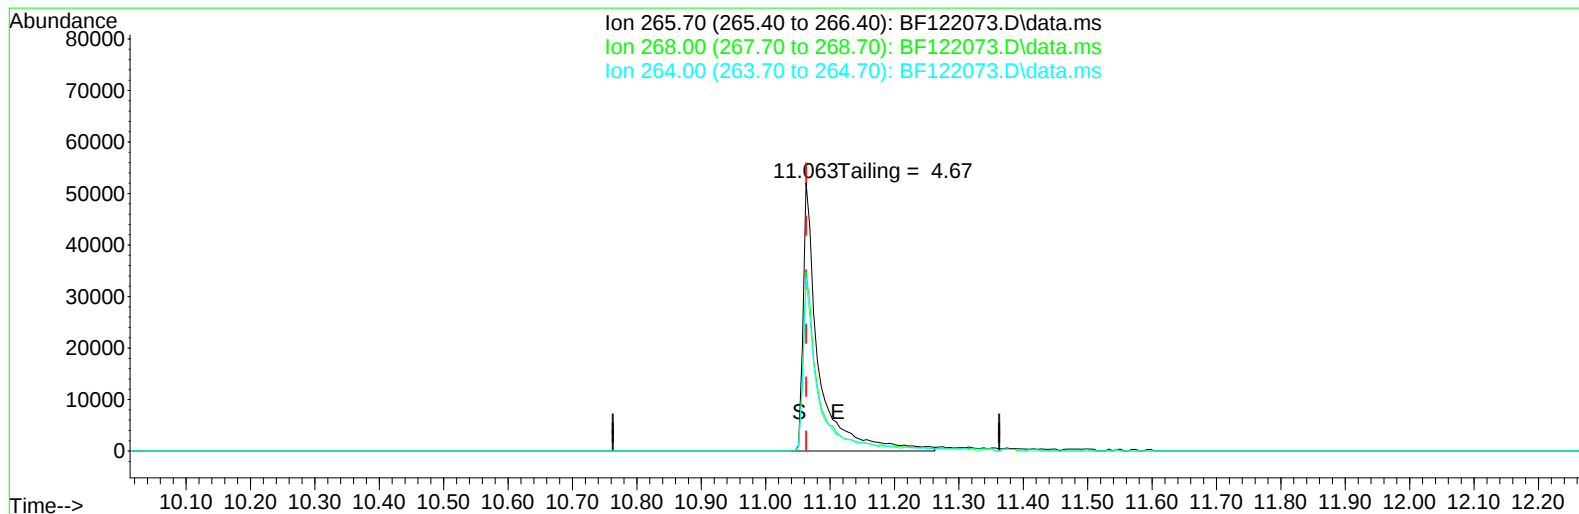

TIC: BF122073.D\data.ms

(70) Pentachlorophenol (C)




11.063min (-0.000) 96933.91 ng

response 87974

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	65.50	66.53
264.00	62.40	64.54
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF102220\
Data File : BF122073.D
Acq On : 22 Oct 2020 9:05
Operator : JU/CG
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 23 04:09:29 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF101220.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Oct 21 12:04:42 2020
Response via : Initial Calibration

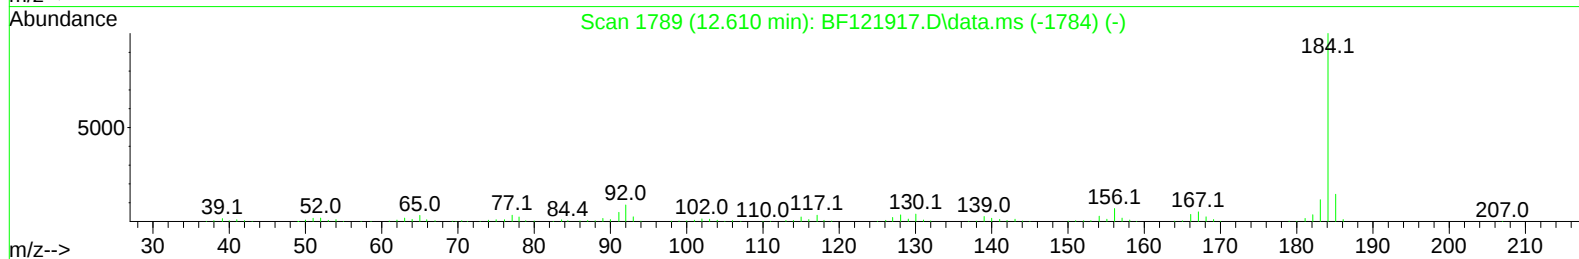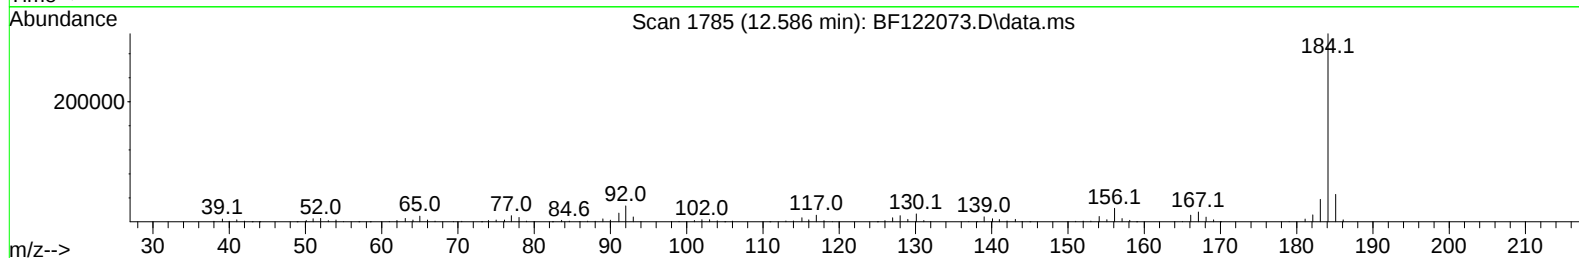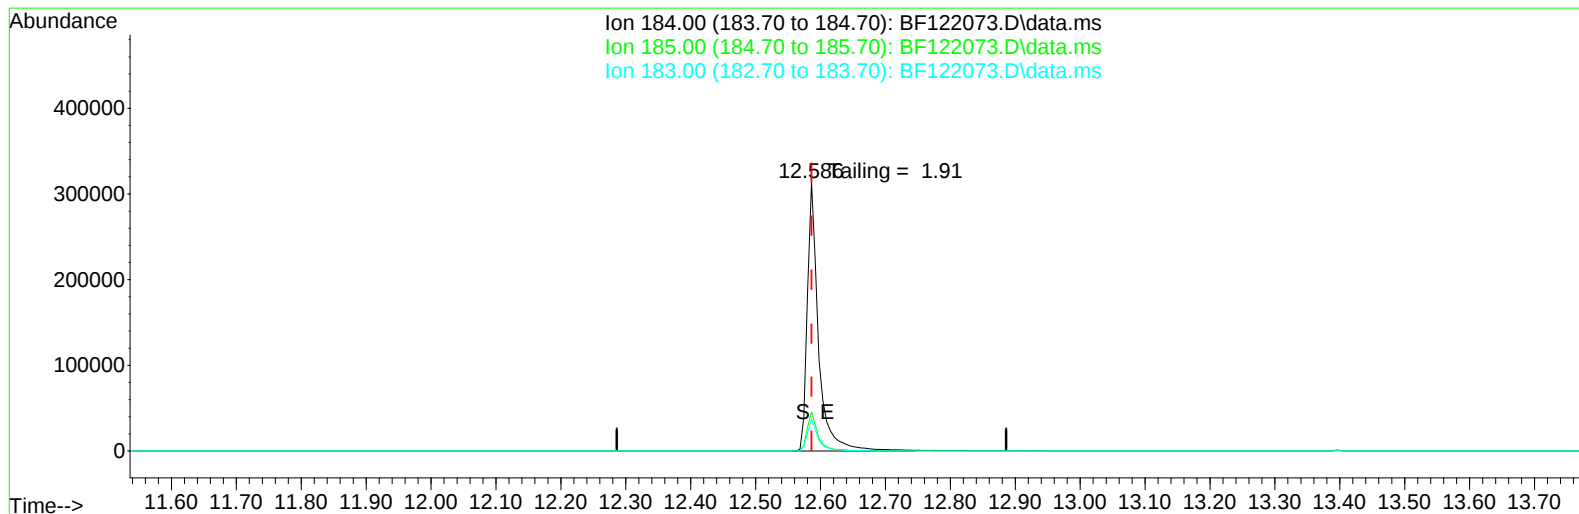

TIC: BF122073.D\data.ms

(77) Benzidine

12.586min (-0.000) 0.00 ng

response 381803

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.50	14.61
183.00	11.70	12.01
0.00	0.00	0.00