

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF102220\
 Data File : BF122075.D
 Acq On : 22 Oct 2020 10:48
 Operator : JU/CG
 Sample : PB132523BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PB132523BL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF101220.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF122075.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	4.975	488	491	504	rBV	34272	62436	1.31%	0.232%
2	5.363	553	557	580	rBV	3174278	3335195	69.99%	12.400%
3	6.381	726	730	758	rBV	2822882	3396174	71.27%	12.627%
4	6.728	786	789	801	rVB	877448	726295	15.24%	2.700%
5	7.298	881	886	889	rBV	2118105	2332649	48.95%	8.673%
6	8.010	1003	1007	1026	rBV	1006367	977942	20.52%	3.636%
7	9.086	1184	1190	1193	rBV	4141717	4026141	84.49%	14.969%
8	9.763	1300	1305	1319	rBV	1103768	1148898	24.11%	4.271%
9	10.557	1435	1440	1467	rBV	2640324	2681271	56.27%	9.969%
10	11.245	1553	1557	1566	rBV	1258056	1208195	25.35%	4.492%
11	12.833	1821	1827	1830	rBV	4405426	4765233	100.00%	17.717%
12	13.886	2002	2006	2018	rVB	1096353	1118386	23.47%	4.158%
13	14.951	2183	2187	2193	rVB	48254	56124	1.18%	0.209%
14	15.321	2244	2250	2267	rVB	627282	1004135	21.07%	3.733%
15	15.715	2312	2317	2322	rVB	39711	57970	1.22%	0.216%




Sum of corrected areas: 26897044

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF102220\
Data File : BF122075.D
Acq On : 22 Oct 2020 10:48
Operator : JU/CG
Sample : PB132523BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB132523BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF101220.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

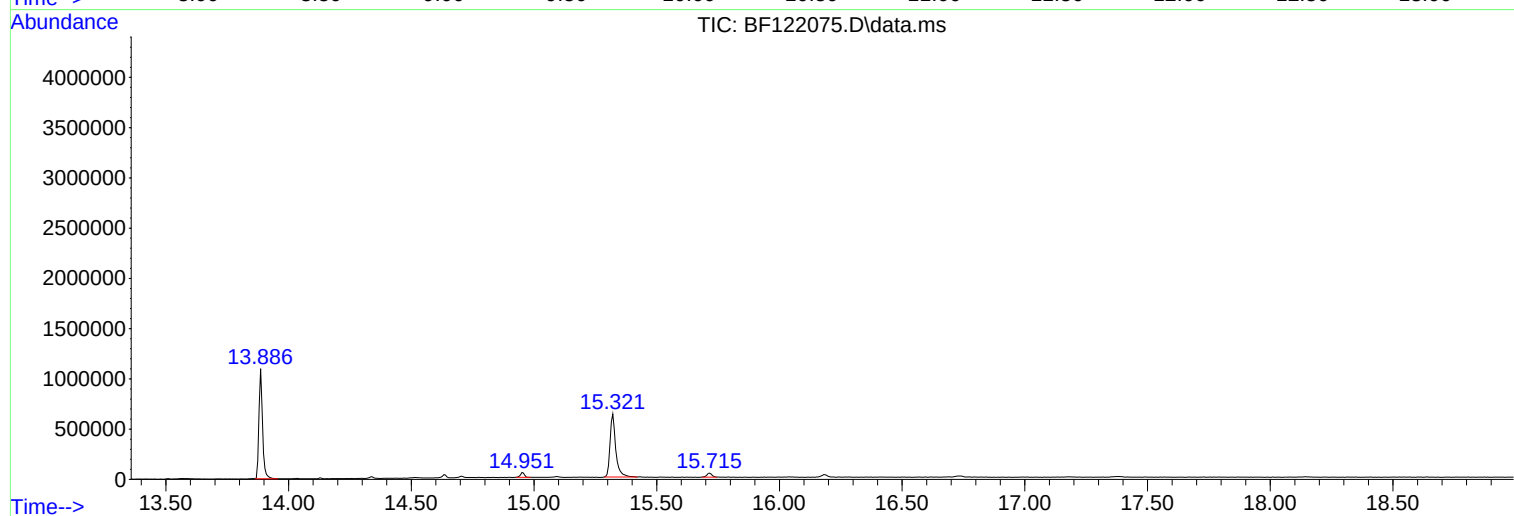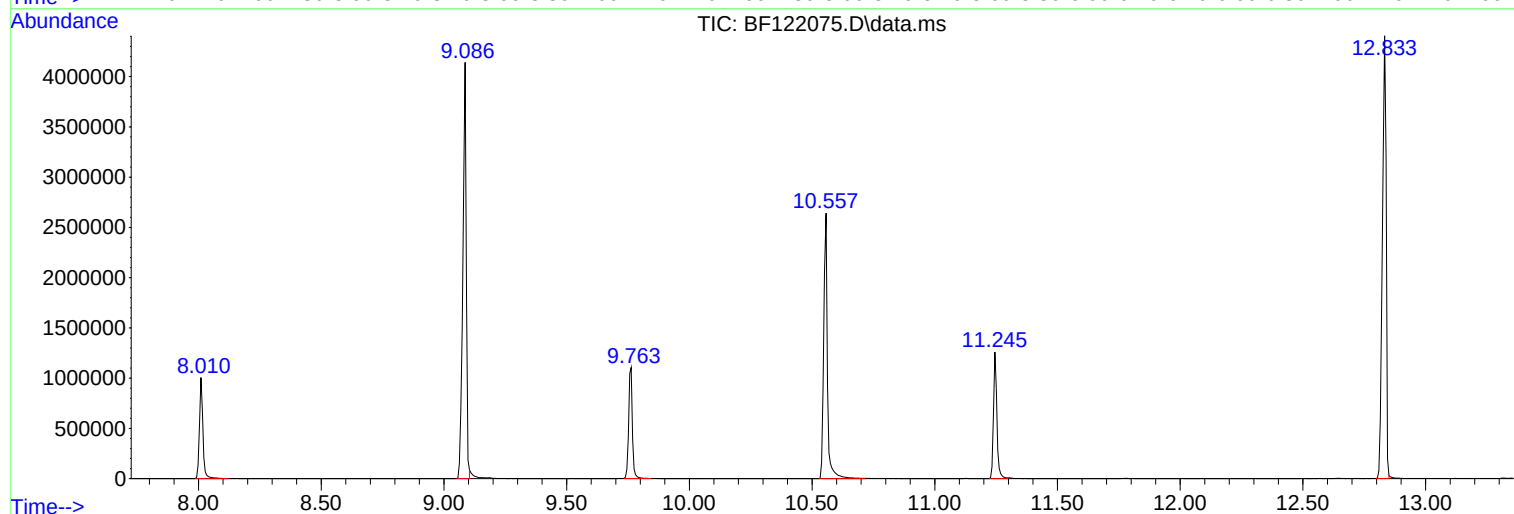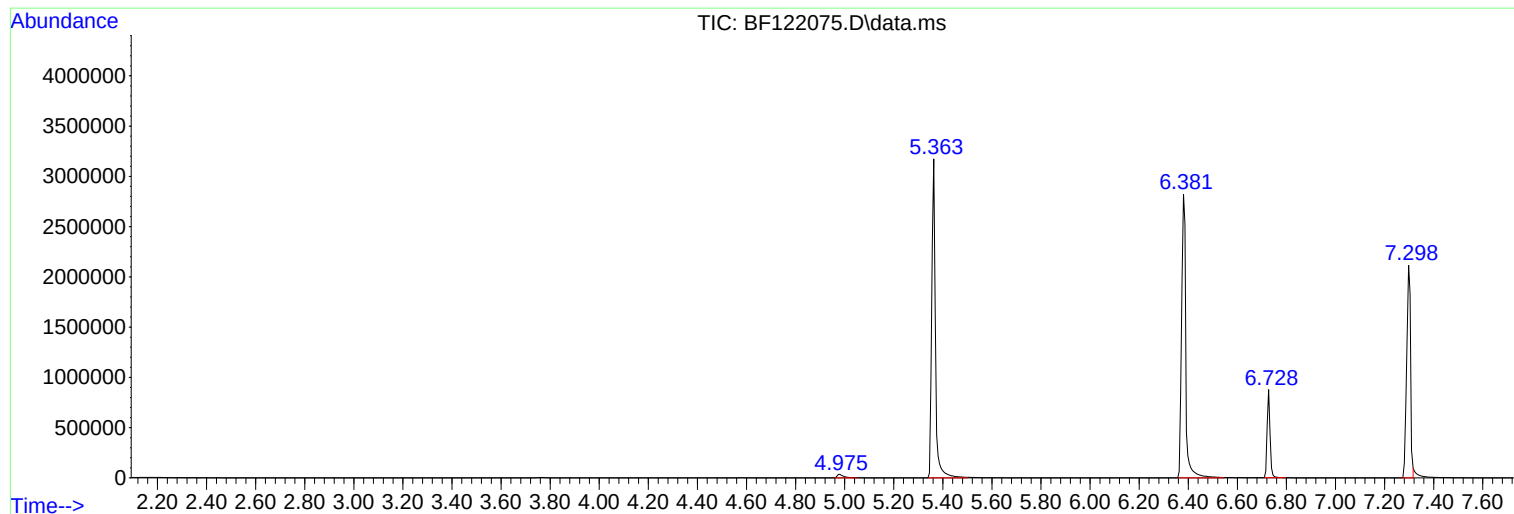

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF102220\
Data File : BF122075.D
Acq On : 22 Oct 2020 10:48
Operator : JU/CG
Sample : PB132523BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB132523BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF101220.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF102220\
Data File : BF122075.D
Acq On : 22 Oct 2020 10:48
Operator : JU/CG
Sample : PB132523BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB132523BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF101220.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------