

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF102220\
 Data File : BF122077.D
 Acq On : 22 Oct 2020 11:48
 Operator : JU/CG
 Sample : PB132482BL
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PB132482BL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF101220.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF122077.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	4.981	488	492	506	rBV	35243	62966	1.29%	0.229%
2	5.363	553	557	580	rBV	3297128	3457365	70.61%	12.576%
3	6.381	726	730	758	rBV	2854783	3537592	72.24%	12.868%
4	6.728	785	789	805	rVB	865908	727964	14.87%	2.648%
5	7.298	881	886	889	rBV	2194263	2435823	49.74%	8.860%
6	8.010	1003	1007	1027	rBV	1045728	992698	20.27%	3.611%
7	9.086	1184	1190	1193	rBV	4231047	4167996	85.12%	15.161%
8	9.757	1300	1304	1325	rVB	1153604	1171673	23.93%	4.262%
9	10.557	1435	1440	1464	rBV	2530560	2757810	56.32%	10.031%
10	11.245	1553	1557	1566	rBV	1220635	1217641	24.87%	4.429%
11	12.833	1822	1827	1830	rBV	4562920	4896767	100.00%	17.811%
12	13.886	2002	2006	2018	rBV	1078019	1107079	22.61%	4.027%
13	15.321	2245	2250	2268	rVB	619052	958995	19.58%	3.488%




Sum of corrected areas: 27492369

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF102220\
Data File : BF122077.D
Acq On : 22 Oct 2020 11:48
Operator : JU/CG
Sample : PB132482BL
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB132482BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF101220.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

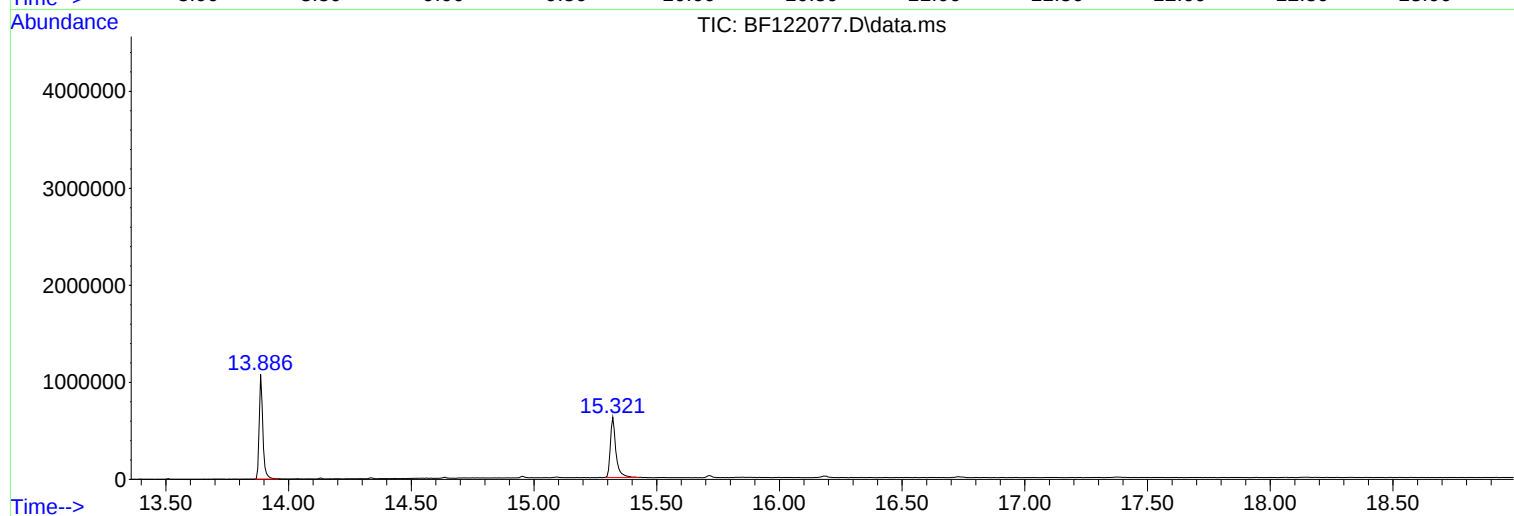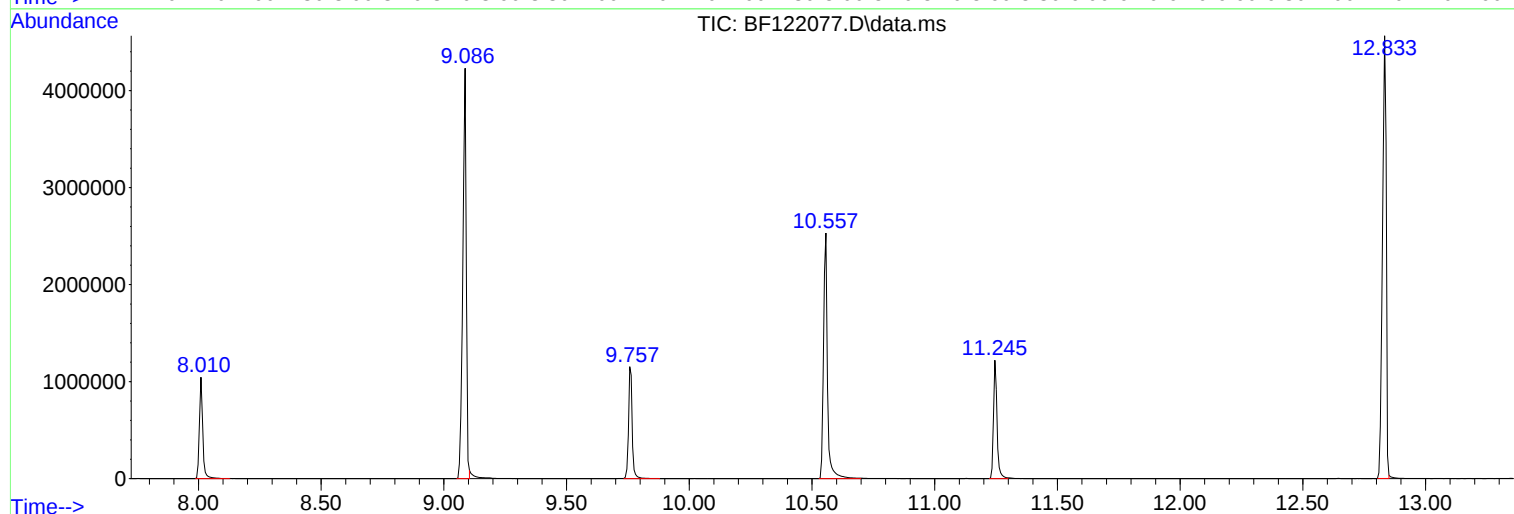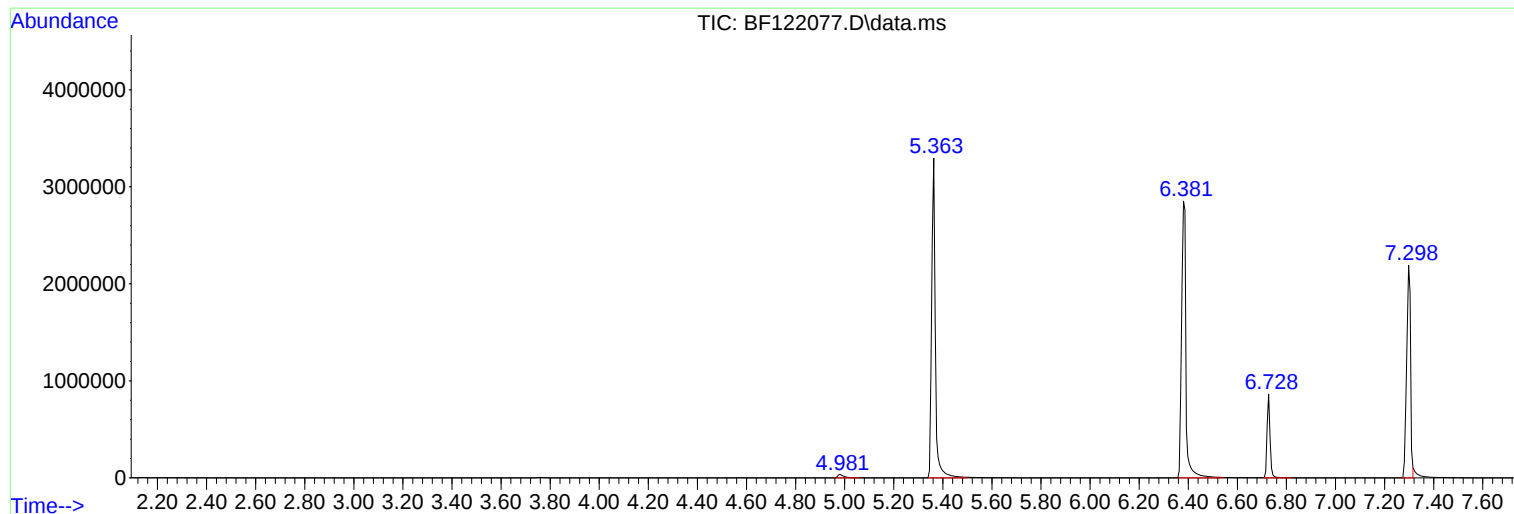

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF102220\
Data File : BF122077.D
Acq On : 22 Oct 2020 11:48
Operator : JU/CG
Sample : PB132482BL
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB132482BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF101220.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF102220\
Data File : BF122077.D
Acq On : 22 Oct 2020 11:48
Operator : JU/CG
Sample : PB132482BL
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB132482BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF101220.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------