

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF102220\
 Data File : BF122089.D
 Acq On : 22 Oct 2020 18:02
 Operator : JU/CG
 Sample : L4436-04
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 34A

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF101220.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF122089.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	4.945	483	486	496	rBV	24847	41655	1.57%	0.207%
2	5.351	552	555	583	rBV	2147804	2342768	88.40%	11.617%
3	6.381	726	730	749	rBV	2217793	2411857	91.01%	11.959%
4	6.586	762	765	775	rBV	22504	46287	1.75%	0.230%
5	6.728	786	789	798	rVB	719188	594650	22.44%	2.949%
6	7.298	882	886	899	rBV	1754269	1657215	62.53%	8.217%
7	8.010	1004	1007	1022	rBV	841191	791922	29.88%	3.927%
8	9.086	1185	1190	1193	rBV	2925256	2650070	100.00%	13.141%
9	9.480	1254	1257	1266	rBV	334621	315046	11.89%	1.562%
10	9.763	1301	1305	1316	rVB	932176	897834	33.88%	4.452%
11	10.551	1436	1439	1455	rBV	1502517	1641721	61.95%	8.141%
12	11.245	1554	1557	1560	rBV	979056	844099	31.85%	4.186%
13	11.269	1560	1561	1565	rVB	152631	111135	4.19%	0.551%
14	11.774	1645	1647	1654	rBV3	83533	92059	3.47%	0.456%
15	11.863	1659	1662	1664	rBV	28858	30477	1.15%	0.151%
16	12.457	1760	1763	1768	rBV	346276	319492	12.06%	1.584%
17	12.686	1797	1802	1807	rBV	274777	317678	11.99%	1.575%
18	12.827	1822	1826	1829	rBV	2422250	2178165	82.19%	10.801%
19	12.904	1836	1839	1844	rBV2	17073	28021	1.06%	0.139%
20	13.051	1860	1864	1867	rBV3	47671	63888	2.41%	0.317%
21	13.121	1874	1876	1883	rVB3	29221	40382	1.52%	0.200%
22	13.392	1919	1922	1925	rBV3	38955	37527	1.42%	0.186%
23	13.539	1944	1947	1950	rBV	28328	30010	1.13%	0.149%
24	13.639	1962	1964	1966	rBV2	30210	30118	1.14%	0.149%
25	13.692	1970	1973	1975	rBV	23823	28205	1.06%	0.140%
26	13.733	1975	1980	1989	rVV4	195977	444410	16.77%	2.204%
27	13.857	1998	2001	2002	rBV	54507	46387	1.75%	0.230%
28	13.886	2002	2006	2009	rVV2	706290	778742	29.39%	3.861%
29	13.915	2009	2011	2017	rVB	155344	143815	5.43%	0.713%
30	14.339	2081	2083	2086	rBV	49651	44519	1.68%	0.221%
31	14.498	2108	2110	2114	rBV	77627	71212	2.69%	0.353%
32	14.915	2178	2181	2184	rBV	145113	182859	6.90%	0.907%
33	15.204	2227	2230	2235	rBV	81975	90271	3.41%	0.448%
34	15.262	2237	2240	2244	rVB	109077	116583	4.40%	0.578%
35	15.321	2246	2250	2254	rBV	472120	589647	22.25%	2.924%
36	16.739	2488	2491	2498	rVB2	68879	116308	4.39%	0.577%

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF102220\
Data File : BF122089.D
Acq On : 22 Oct 2020 18:02
Operator : JU/CG
Sample : L4436-04
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
34A

Integration Parameters: rteint.p
Integrator: RTE
Smoothing : ON Filtering: 5
Sampling : 1 Min Area: 3 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF101220.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION




Sum of corrected areas: 20167034

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF102220\
Data File : BF122089.D
Acq On : 22 Oct 2020 18:02
Operator : JU/CG
Sample : L4436-04
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampled :
34A

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF10220.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library :
TIC Integration Parameters: rteint.p

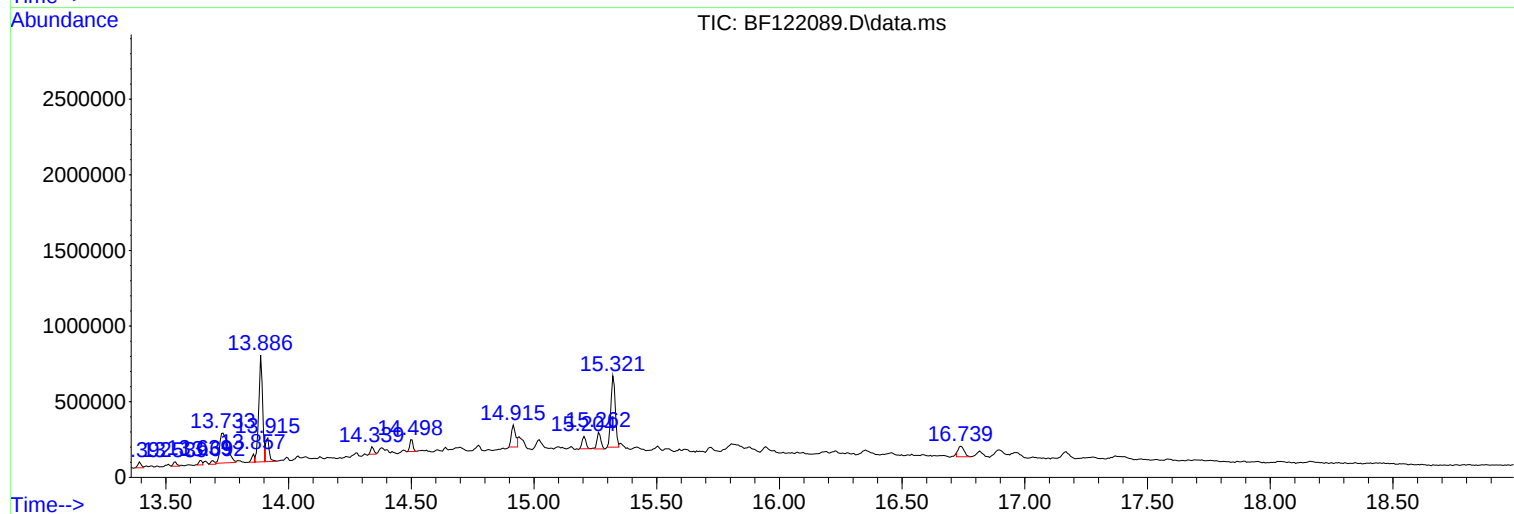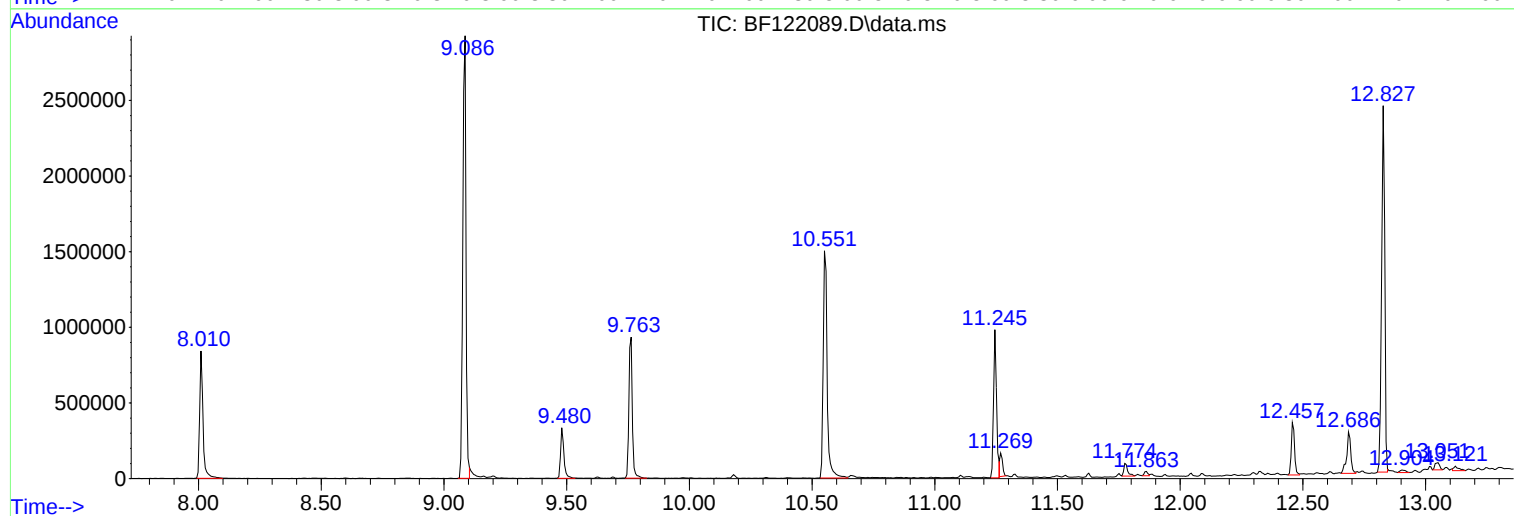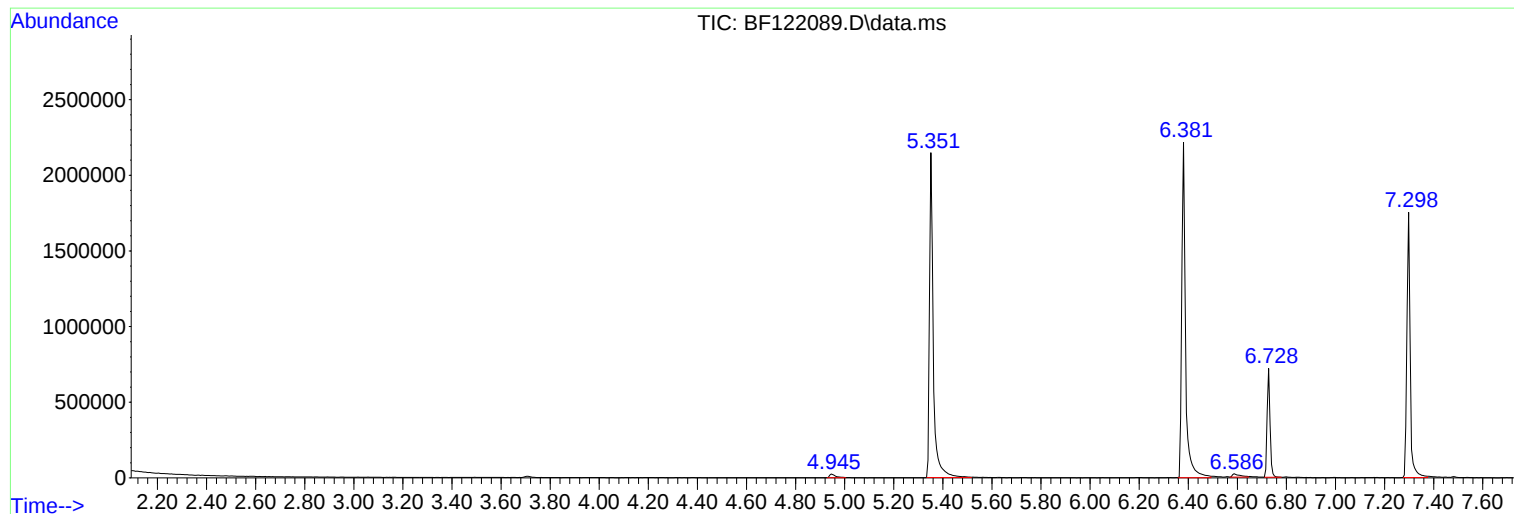

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF102220\
Data File : BF122089.D
Acq On : 22 Oct 2020 18:02
Operator : JU/CG
Sample : L4436-04
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
34A

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF101220.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library :
TIC Integration Parameters: rteint.p

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF102220\
Data File : BF122089.D
Acq On : 22 Oct 2020 18:02
Operator : JU/CG
Sample : L4436-04
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
34A

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF101220.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library :
TIC Integration Parameters: rteint.p

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------