

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF102220\
 Data File : BF122094.D
 Acq On : 22 Oct 2020 20:36
 Operator : JU/CG
 Sample : L4436-11 10X
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 37B

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF101220.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF122094.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.369	555	558	576	rBV	82749	166166	22.31%	3.248%
2	6.398	731	733	756	rBV	72292	176787	23.74%	3.456%
3	6.728	786	789	809	rVB	604915	547682	73.54%	10.705%
4	7.304	884	887	907	rBV	72389	121762	16.35%	2.380%
5	8.010	1004	1007	1024	rBV	637389	671815	90.21%	13.132%
6	9.086	1186	1190	1201	rBV	145689	171442	23.02%	3.351%
7	9.486	1254	1258	1265	rBV	12970	16140	2.17%	0.315%
8	9.763	1301	1305	1320	rBV	675221	657238	88.26%	12.847%
9	10.563	1437	1441	1450	rBV	63506	76352	10.25%	1.492%
10	11.251	1554	1558	1561	rBV	555599	579886	77.87%	11.335%
11	11.327	1569	1571	1576	rVB	11193	10542	1.42%	0.206%
12	11.780	1646	1648	1654	rVB	9807	10936	1.47%	0.214%
13	11.863	1660	1662	1665	rBV	10735	10538	1.42%	0.206%
14	12.304	1733	1737	1739	rBV	6911	8588	1.15%	0.168%
15	12.463	1761	1764	1770	rBV	111304	98184	13.18%	1.919%
16	12.692	1797	1803	1809	rBV	106250	114373	15.36%	2.236%
17	12.827	1822	1826	1830	rBV	186715	165163	22.18%	3.228%
18	12.916	1836	1841	1845	rBV3	8130	13073	1.76%	0.256%
19	13.022	1853	1859	1862	rBV2	13502	20065	2.69%	0.392%
20	13.086	1868	1870	1872	rBV2	8487	8801	1.18%	0.172%
21	13.251	1895	1898	1900	rBV2	8846	7790	1.05%	0.152%
22	13.751	1981	1983	1988	rBB5	14568	14851	1.99%	0.290%
23	13.892	2002	2007	2010	rBV	701428	744694	100.00%	14.556%
24	14.915	2179	2181	2184	rBV	39947	43456	5.84%	0.849%
25	15.268	2238	2241	2245	rVB	35089	40770	5.47%	0.797%
26	15.327	2246	2251	2260	rBV	481708	618827	83.10%	12.096%




Sum of corrected areas: 5115921

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF102220\
Data File : BF122094.D
Acq On : 22 Oct 2020 20:36
Operator : JU/CG
Sample : L4436-11 10X
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
37B

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF101220.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

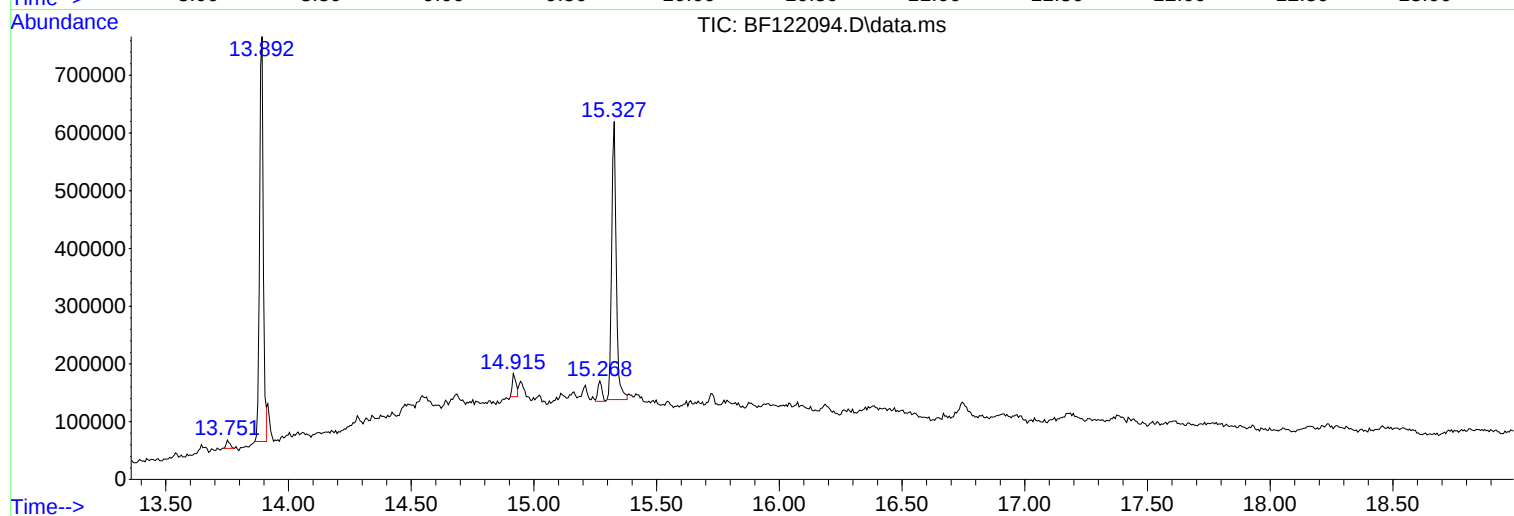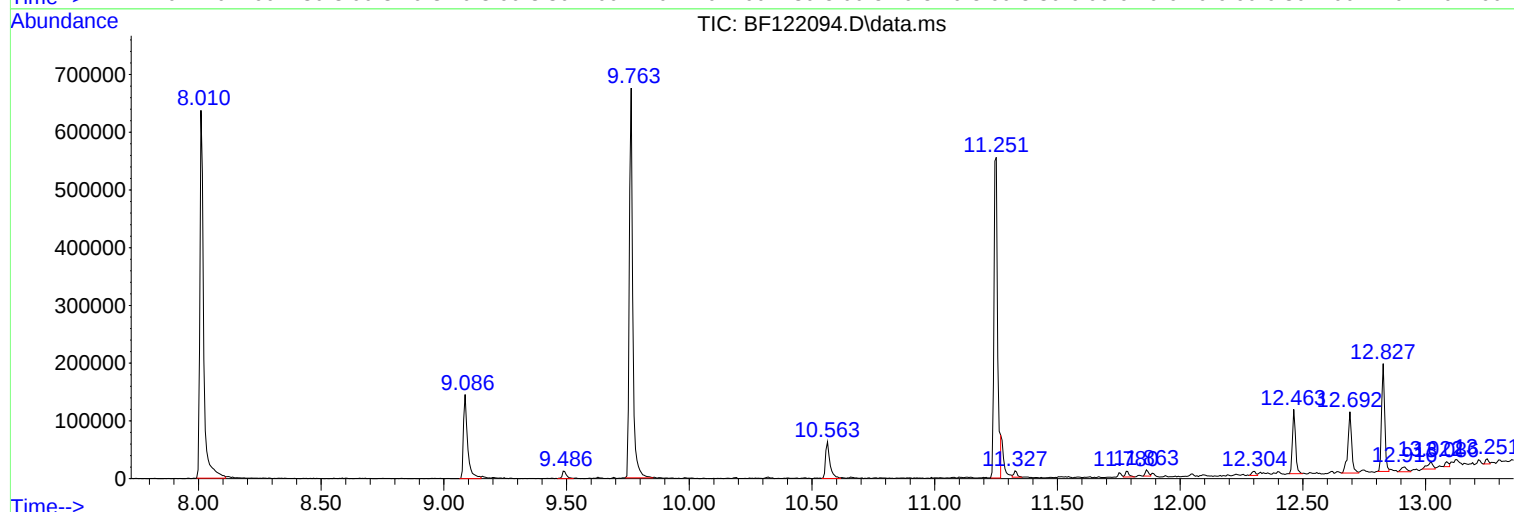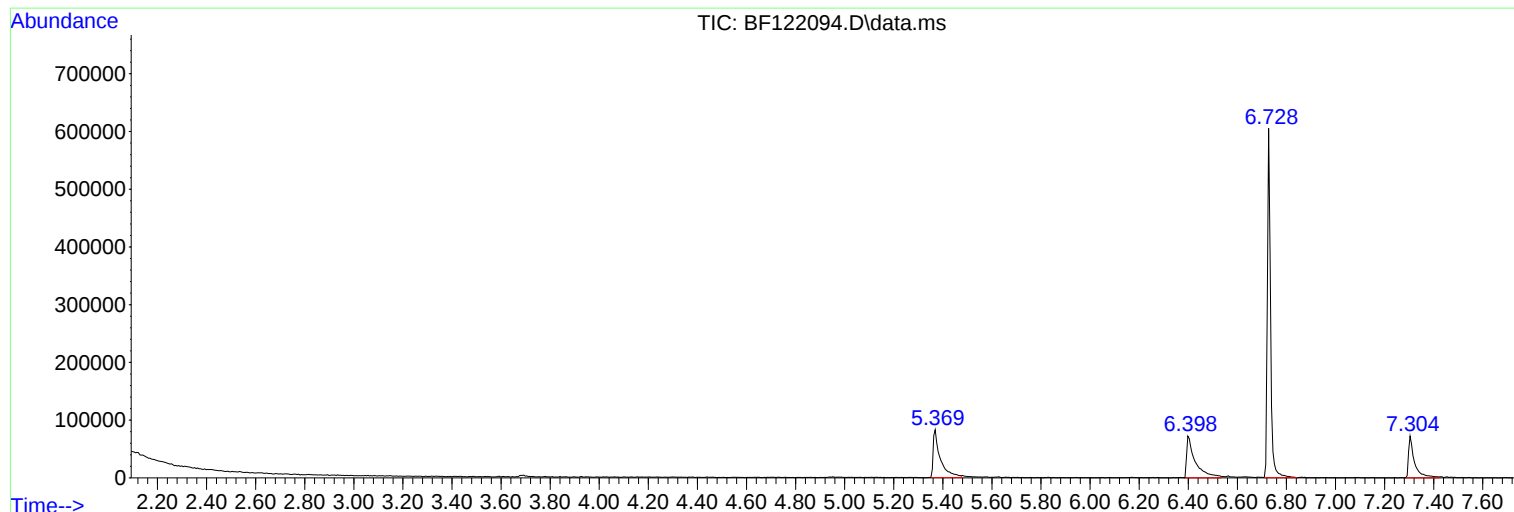

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF102220\
Data File : BF122094.D
Acq On : 22 Oct 2020 20:36
Operator : JU/CG
Sample : L4436-11 10X
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
37B

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF101220.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF102220\
Data File : BF122094.D
Acq On : 22 Oct 2020 20:36
Operator : JU/CG
Sample : L4436-11 10X
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
37B

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF101220.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
