
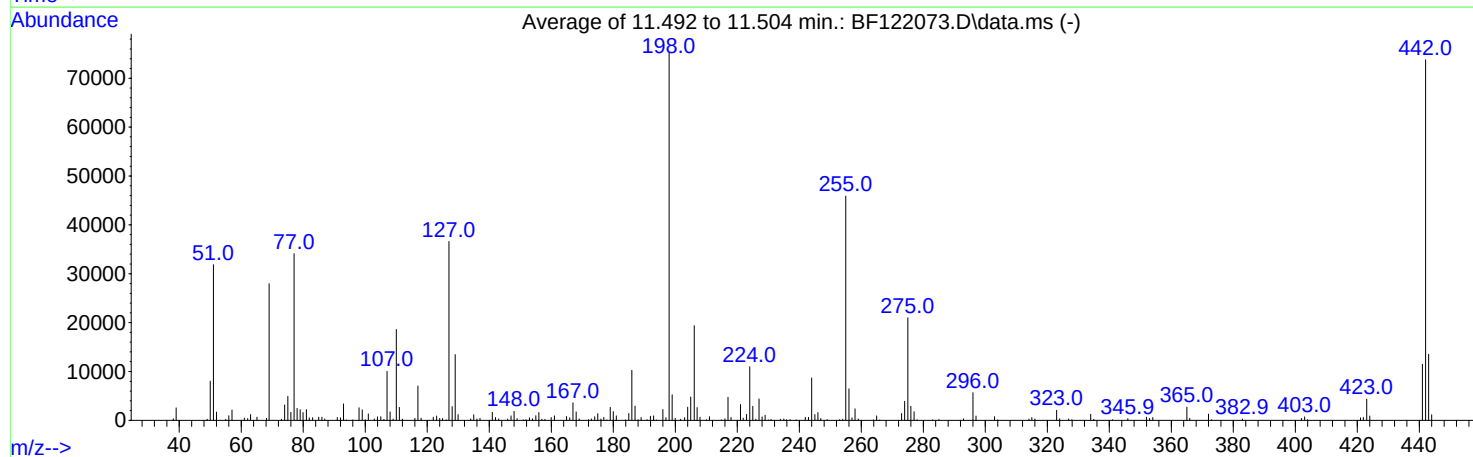


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF102220\
 Data File : BF122073.D
 Acq On : 22 Oct 2020 9:05
 Operator : JU/CG
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF101220.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Oct 21 12:04:42 2020

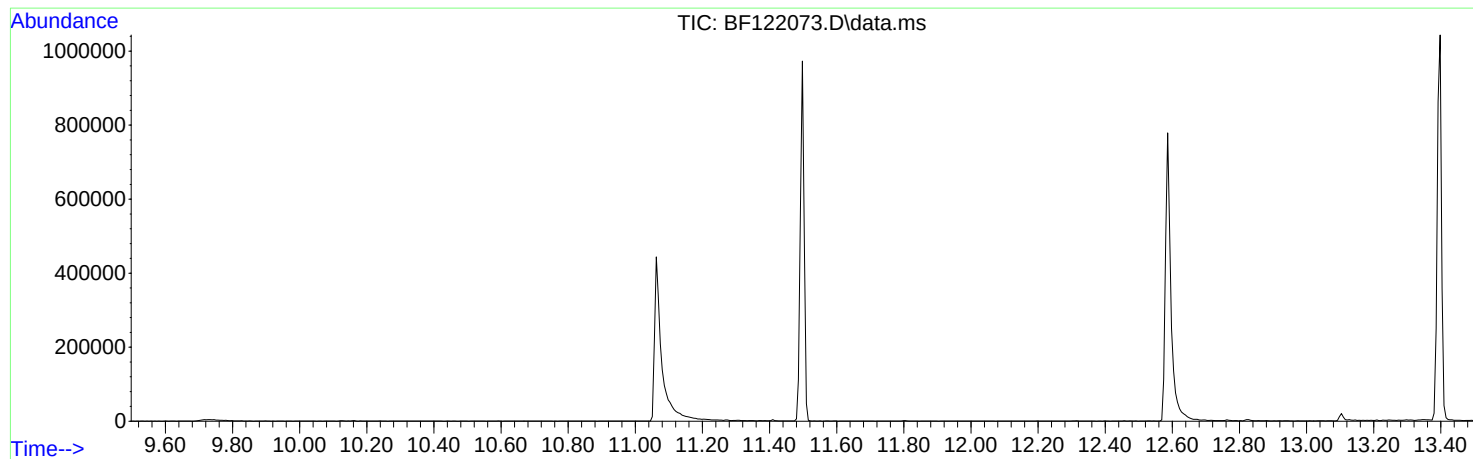

AutoFind: Scans 1599, 1600, 1601; Background Corrected with Scan 1594

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	42.3	31862	PASS
68	69	0.00	2	1.5	416	PASS
69	198	0.00	100	37.1	27944	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	48.6	36592	PASS
197	198	0.00	2	0.7	551	PASS
198	198	100	100	100.0	75267	PASS
199	198	5	9	7.0	5248	PASS
275	198	10	60	27.9	20974	PASS
365	198	1	100	3.6	2725	PASS
441	198	0.01	100	15.3	11508	PASS
442	198	50	100	98.0	73776	PASS
443	442	15	24	18.3	13533	PASS