
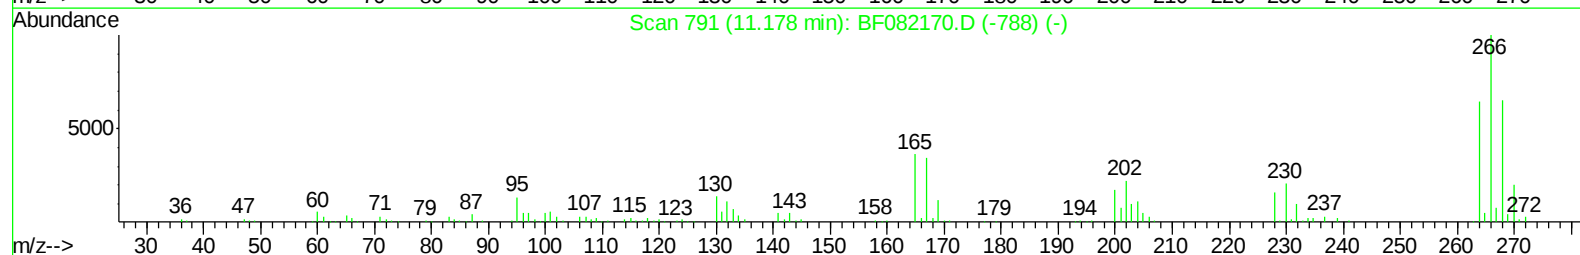
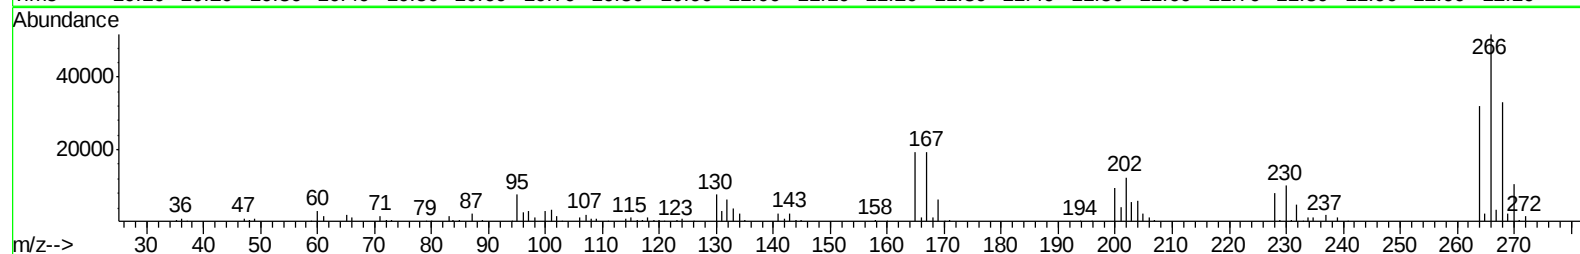


Data Path : Z:\HPCHEM1\BNA\_F\DATA\BF102315\  
Data File : BF082469.D  
Acq On : 23 Oct 2015 16:05  
Operator : UM/IZ  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 23 16:32:29 2015  
Quant Method : Z:\HPCHEM1\BNA\_F\METHODS\8270-BF101015.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Wed Oct 21 13:20:24 2015  
Response via : Initial Calibration

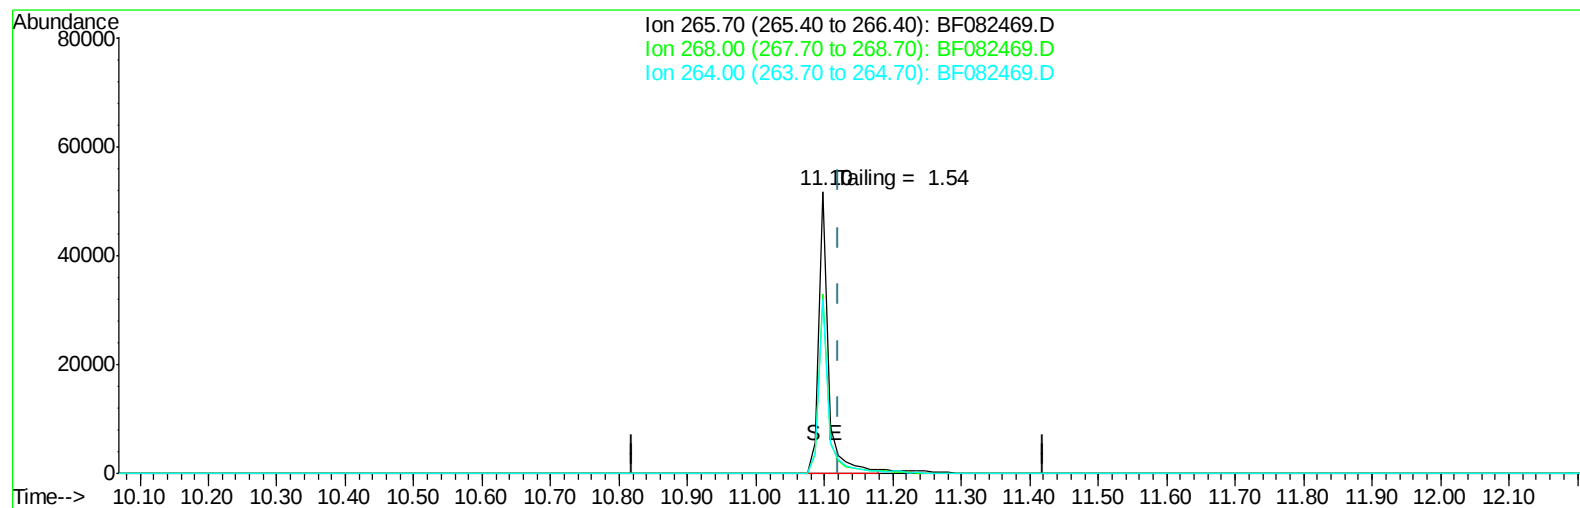

TIC: BF082469.D

(69) Pentachlorophenol (C)




11.098min (-0.023) 0.00ng

response 52754

| Ion    | Exp%  | Act%  |
|--------|-------|-------|
| 265.70 | 100   | 100   |
| 268.00 | 65.00 | 63.87 |
| 264.00 | 64.20 | 61.78 |
| 0.00   | 0.00  | 0.00  |

Data Path : Z:\HPCHEM1\BNA\_F\DATA\BF102315\  
Data File : BF082469.D  
Acq On : 23 Oct 2015 16:05  
Operator : UM/IZ  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 23 16:32:29 2015  
Quant Method : Z:\HPCHEM1\BNA\_F\METHODS\8270-BF101015.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Wed Oct 21 13:20:24 2015  
Response via : Initial Calibration

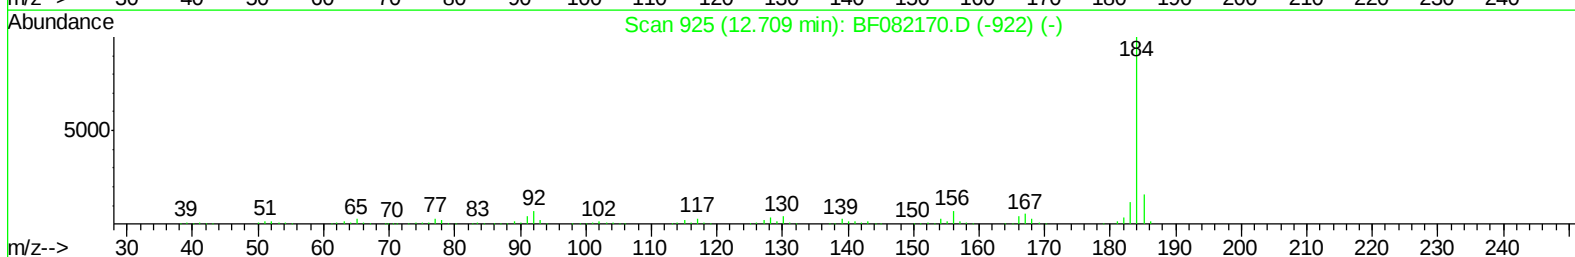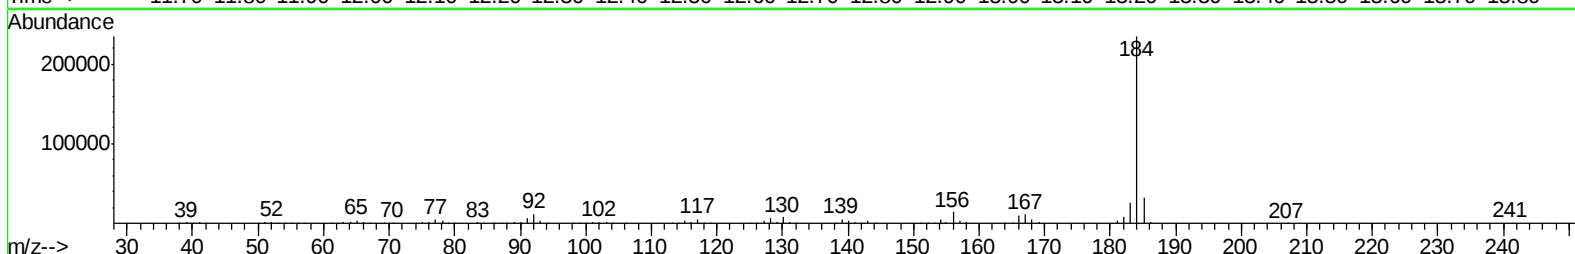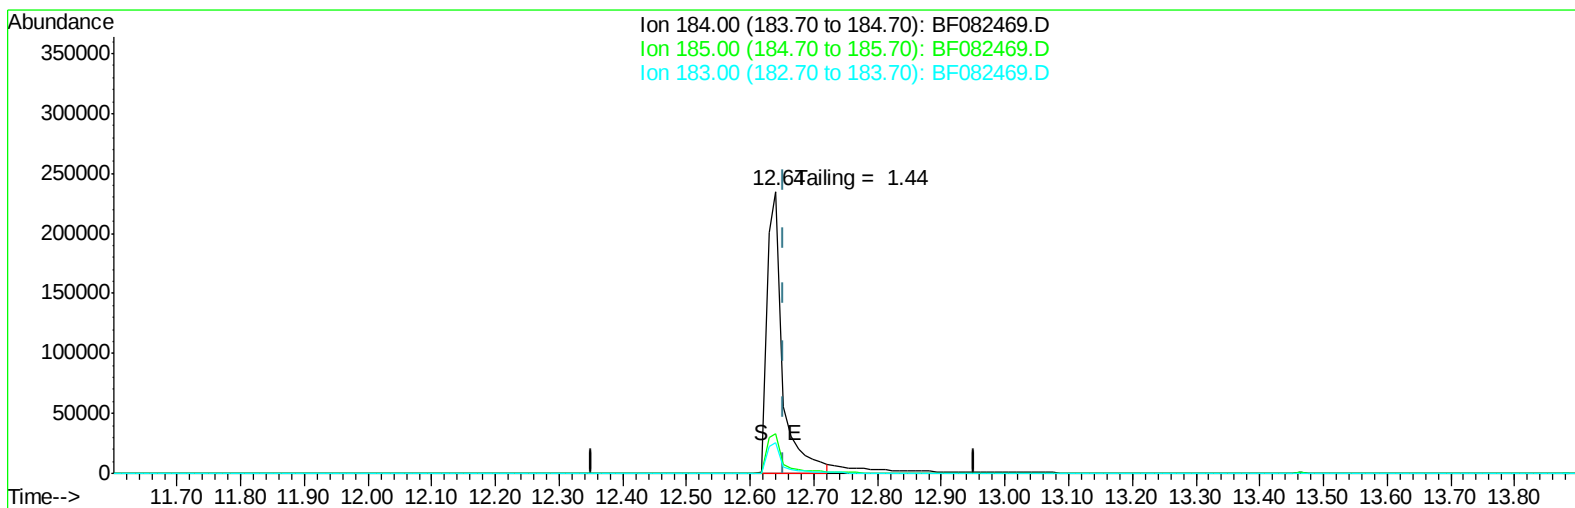

TIC: BF082469.D

(76) Benzidine

12.641min (-0.011) 0.00ng

response 435907

| Ion    | Exp%  | Act%  |
|--------|-------|-------|
| 184.00 | 100   | 100   |
| 185.00 | 15.60 | 14.01 |
| 183.00 | 11.40 | 10.95 |
| 0.00   | 0.00  | 0.00  |