
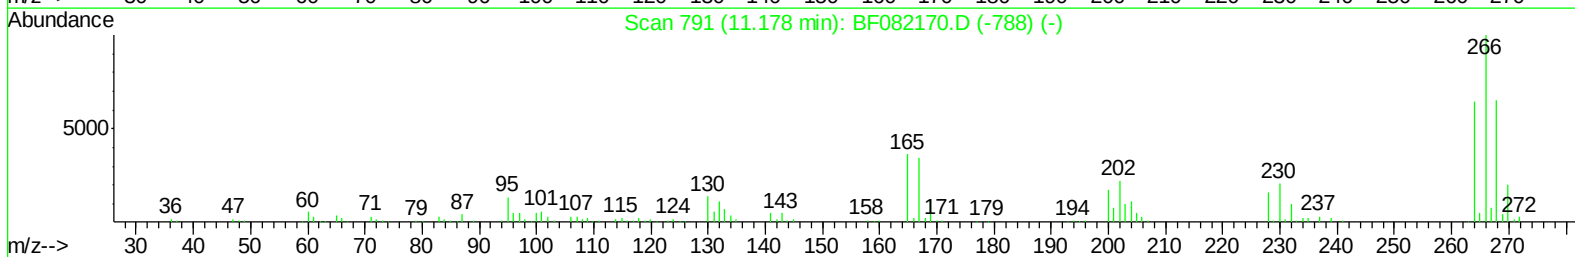
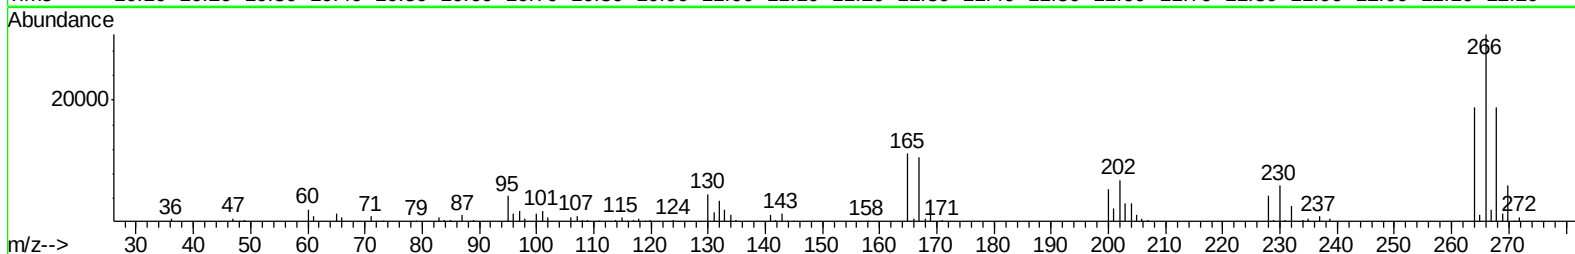


Data Path : Z:\HPCHEM1\BNA_F\DATA\BF102315\
Data File : BF082493.D
Acq On : 24 Oct 2015 5:19
Operator : UM/IZ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 26 19:55:19 2015
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF101015.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Oct 23 15:17:13 2015
Response via : Initial Calibration

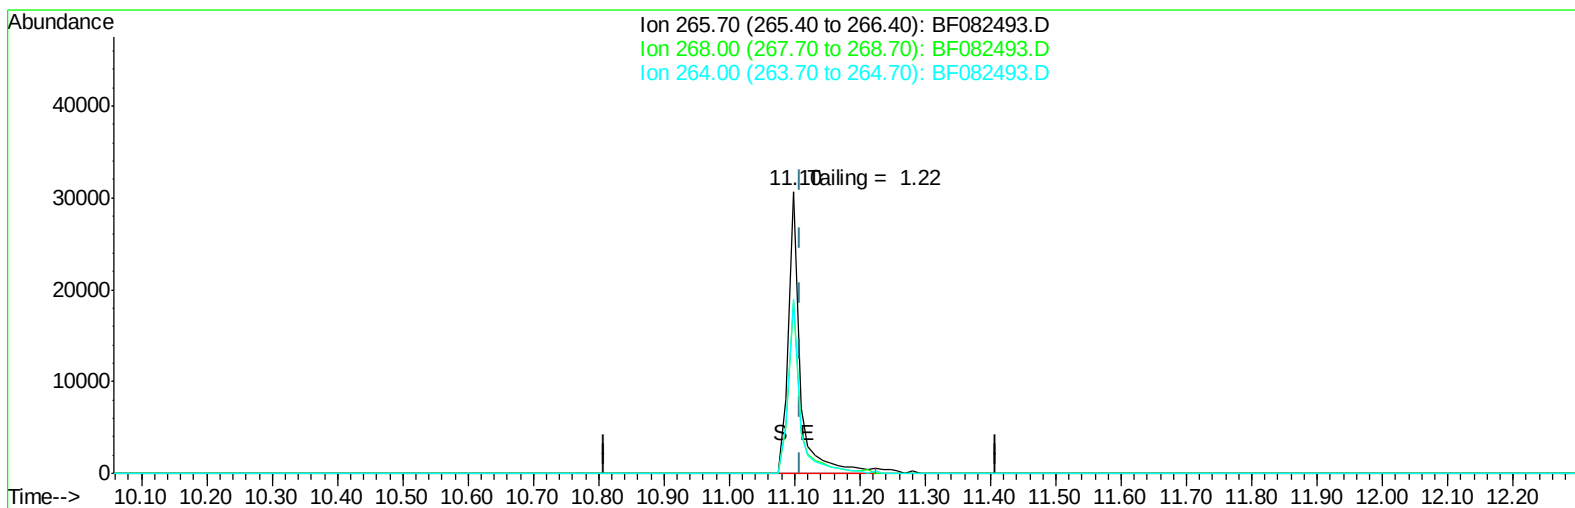

TIC: BF082493.D

(69) Pentachlorophenol (C)




11.098min (-0.011) 0.00ng

response 40028

Ion	Exp%	Act%
265.70	100	100
268.00	65.00	61.13
264.00	64.20	61.70
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF102315\
Data File : BF082493.D
Acq On : 24 Oct 2015 5:19
Operator : UM/IZ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 26 19:55:19 2015
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF101015.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Oct 23 15:17:13 2015
Response via : Initial Calibration

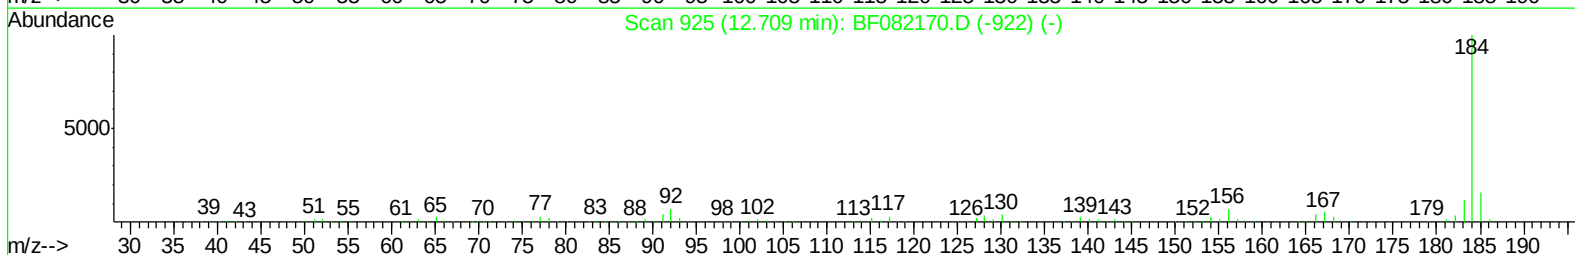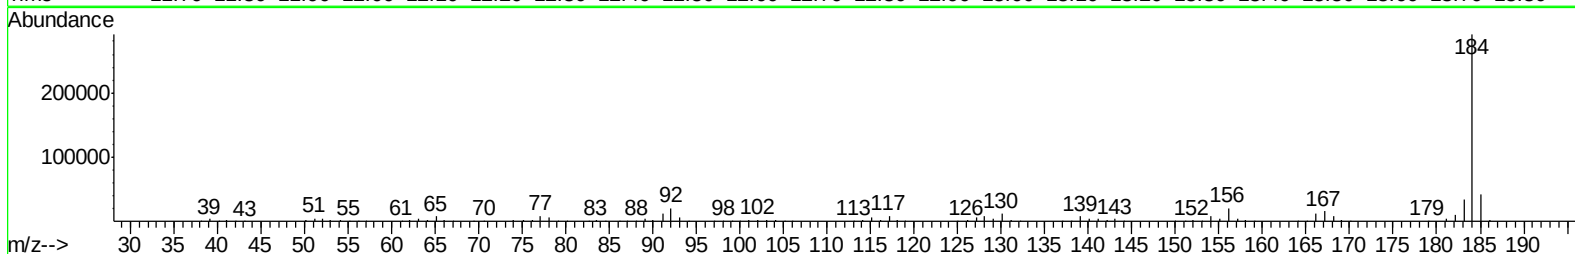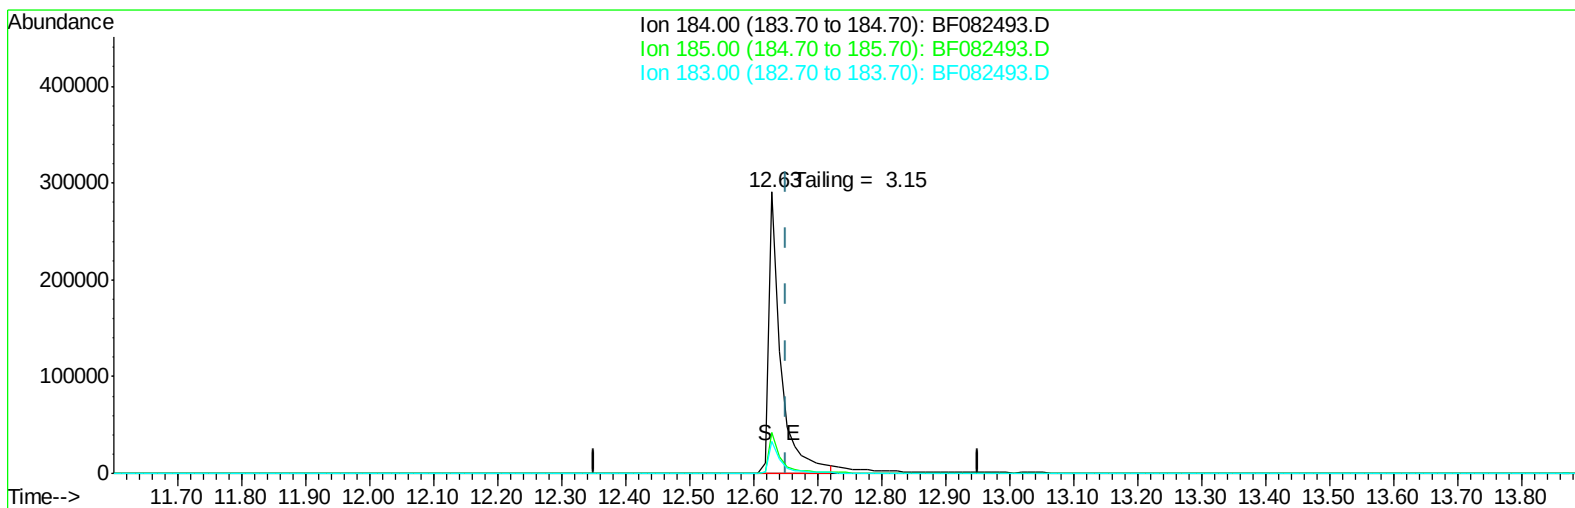

TIC: BF082493.D

(76) Benzidine

12.629min (-0.023) 0.00ng

response 416813

Ion	Exp%	Act%
184.00	100	100
185.00	15.60	14.54
183.00	11.40	11.47
0.00	0.00	0.00