

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF102315\
Data File : BF082478.D
Acq On : 23 Oct 2015 21:21
Operator : UM/IZ
Sample : PB86220BL
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB86220BL

Integration Parameters: rteint.p
Integrator: RTE
Smoothing : ON Filtering: 5
Sampling : 1 Min Area: 3 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF101015.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	4.926	240	244	253	rBV	682009	1221520	38.02%	5.701%
2	5.360	279	282	284	rBV	1511682	1941906	60.44%	9.062%
3	6.400	370	373	376	rBV	1758740	1778109	55.34%	8.298%
4	6.526	381	384	386	rBV	1756488	2092510	65.13%	9.765%
5	6.754	402	404	406	rBV	418020	473704	14.74%	2.211%
6	6.903	415	417	420	rBV	1676886	1608572	50.07%	7.507%
7	7.326	451	454	456	rBV	1178613	1277392	39.76%	5.961%
8	8.034	514	516	519	rBV	503573	626168	19.49%	2.922%
9	9.120	608	611	614	rBV	2501168	2575457	80.16%	12.019%
10	9.795	667	670	673	rBV	828005	798442	24.85%	3.726%
11	10.595	737	740	742	rBV	1125318	1493089	46.47%	6.968%
12	11.281	798	800	803	rBV	810157	814050	25.34%	3.799%
13	12.881	937	940	942	rBV	2880301	3212830	100.00%	14.993%
14	13.932	1030	1032	1035	rBV	707401	819110	25.49%	3.823%
15	15.395	1157	1160	1167	rBV	474380	695377	21.64%	3.245%


Sum of corrected areas: 21428236

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF102315\
Data File : BF082478.D
Acq On : 23 Oct 2015 21:21
Operator : UM/IZ
Sample : PB86220BL
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB86220BL

Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF101015.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

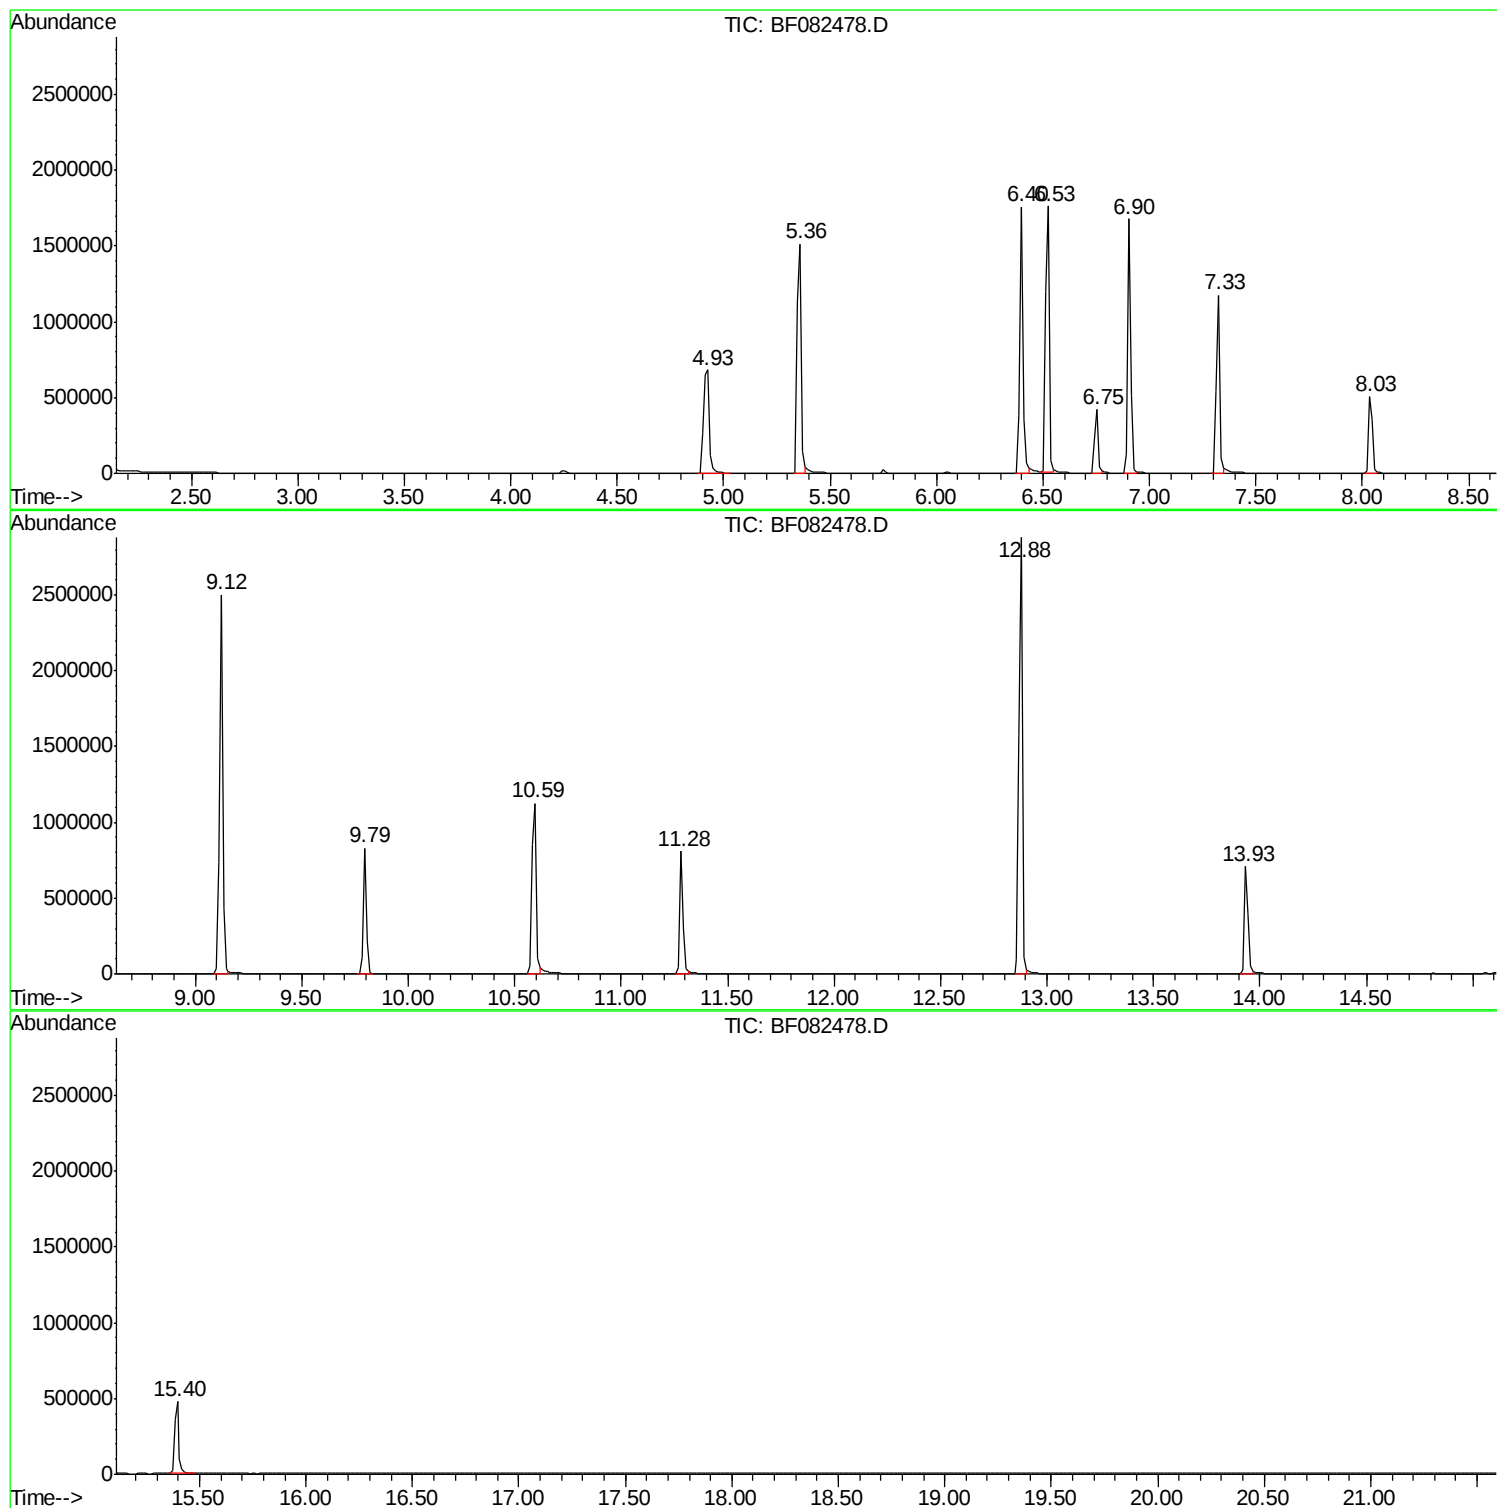

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF102315\
Data File : BF082478.D
Acq On : 23 Oct 2015 21:21
Operator : UM/IZ
Sample : PB86220BL
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB86220BL










Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF101015.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 2-Pentanone, 4-hydroxy-4-me... Concentration Rank 3

R.T.	EstConc	Area	Relative to ISTD	R.T.
4.93	51.57 ng	1221520	1,4-Dichlorobenzene-d4	6.75

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	2-Pentanone, 4-hydroxy-4-methyl-	116	C6H12O2	000123-42-2	56
2		Propane, 2-methyl-2-(1-methyleth...	116	C7H16O	017348-59-3	53
3		Acetic acid, cyano-, 1,1-dimethy...	141	C7H11NO2	001116-98-9	17
4		Morpholine, 4-methyl-	101	C5H11NO	000109-02-4	9
5		Guanidine	59	CH5N3	000113-00-8	9

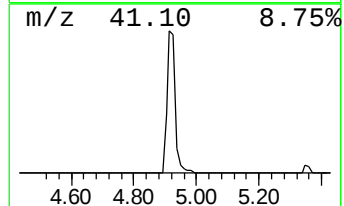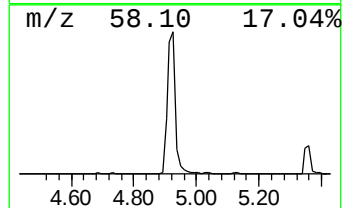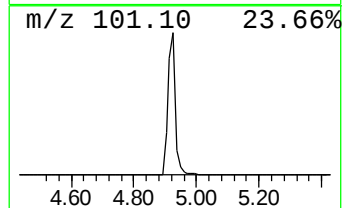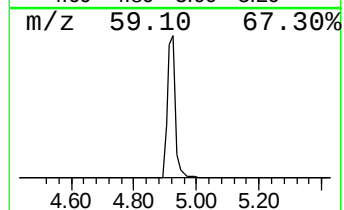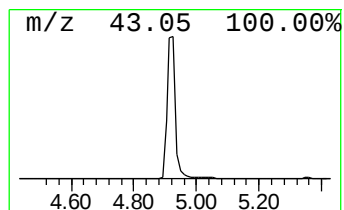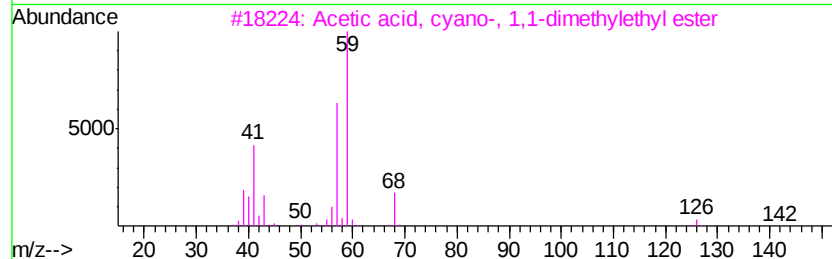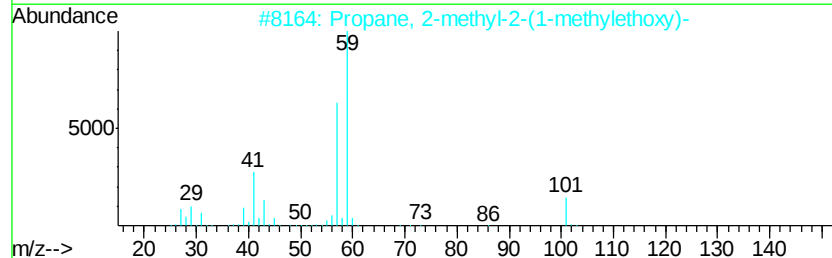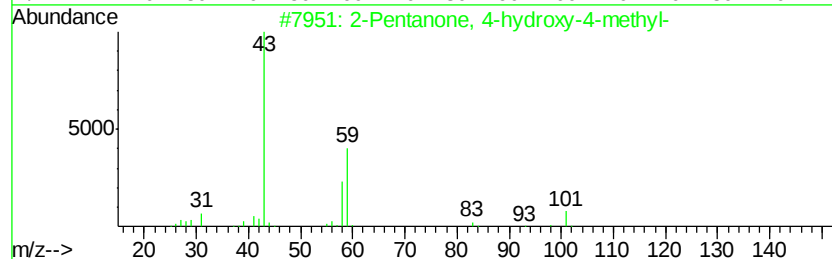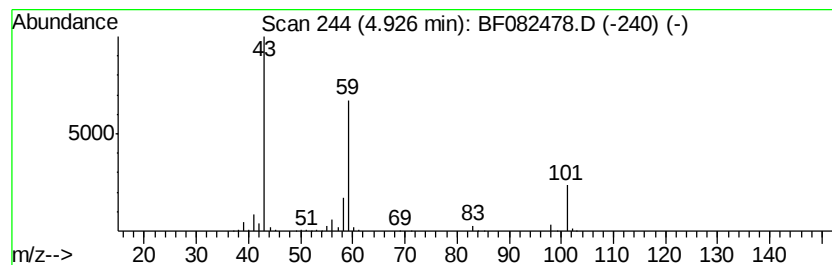

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF102315\
Data File : BF082478.D
Acq On : 23 Oct 2015 21:21
Operator : UM/IZ
Sample : PB86220BL
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB86220BL










Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF101015.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

Peak Number 2 unknown6.53 Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
6.53	88.35 ng	2092510	1,4-Dichlorobenzene-d4	6.75

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	3-Chloro-6-fluoro-pyrazine	132	C4H2ClFN2	1000146-10-7	38
2		(E)-3-Chloro-2-methyl-2-pentenal	132	C6H9ClO	031357-76-3	16
3		Amphetaminil	250	C17H18N2	017590-01-1	12
4		Tranlylcypromine-propionyl	189	C12H15NO	1000123-86-3	12
5		5-Aminoindole	132	C8H8N2	005192-03-0	12

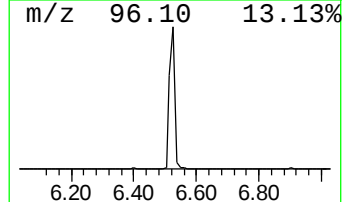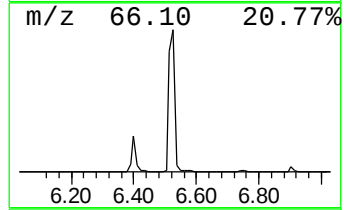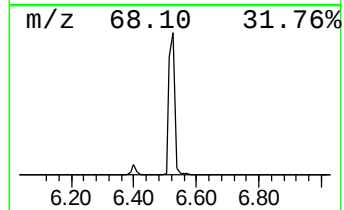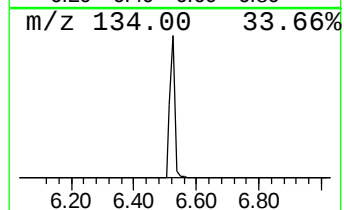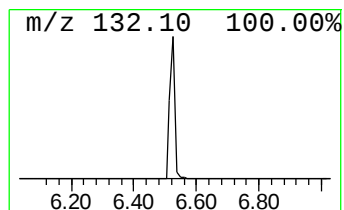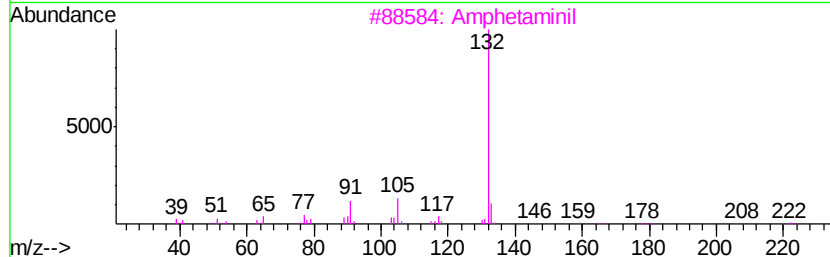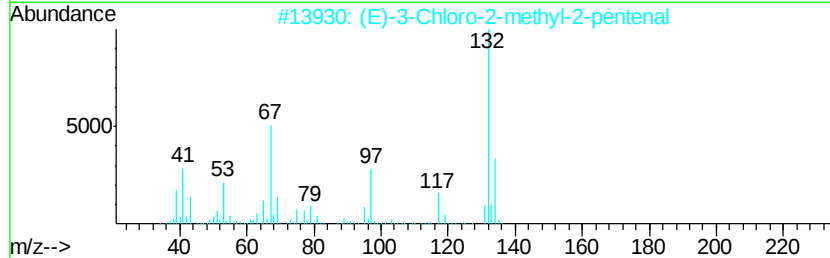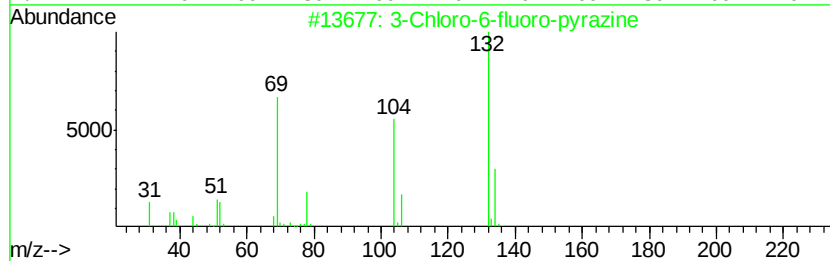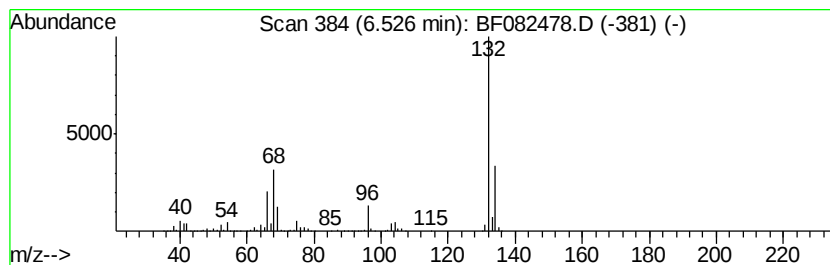

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF102315\
Data File : BF082478.D
Acq On : 23 Oct 2015 21:21
Operator : UM/IZ
Sample : PB86220BL
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB86220BL

Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF101015.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
2-Pentanone, 4-hy...	4.93	51.6	ng	1221520	1	6.75	473704	20.0
unknown6.53	6.53	88.3	ng	2092510	1	6.75	473704	20.0