


Data Path : Z:\HPCHEM1\BNA_F\DATA\BF102315\
 Data File : BF082469.D
 Acq On : 23 Oct 2015 16:05
 Operator : UM/IZ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF101015.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Oct 23 15:17:13 2015

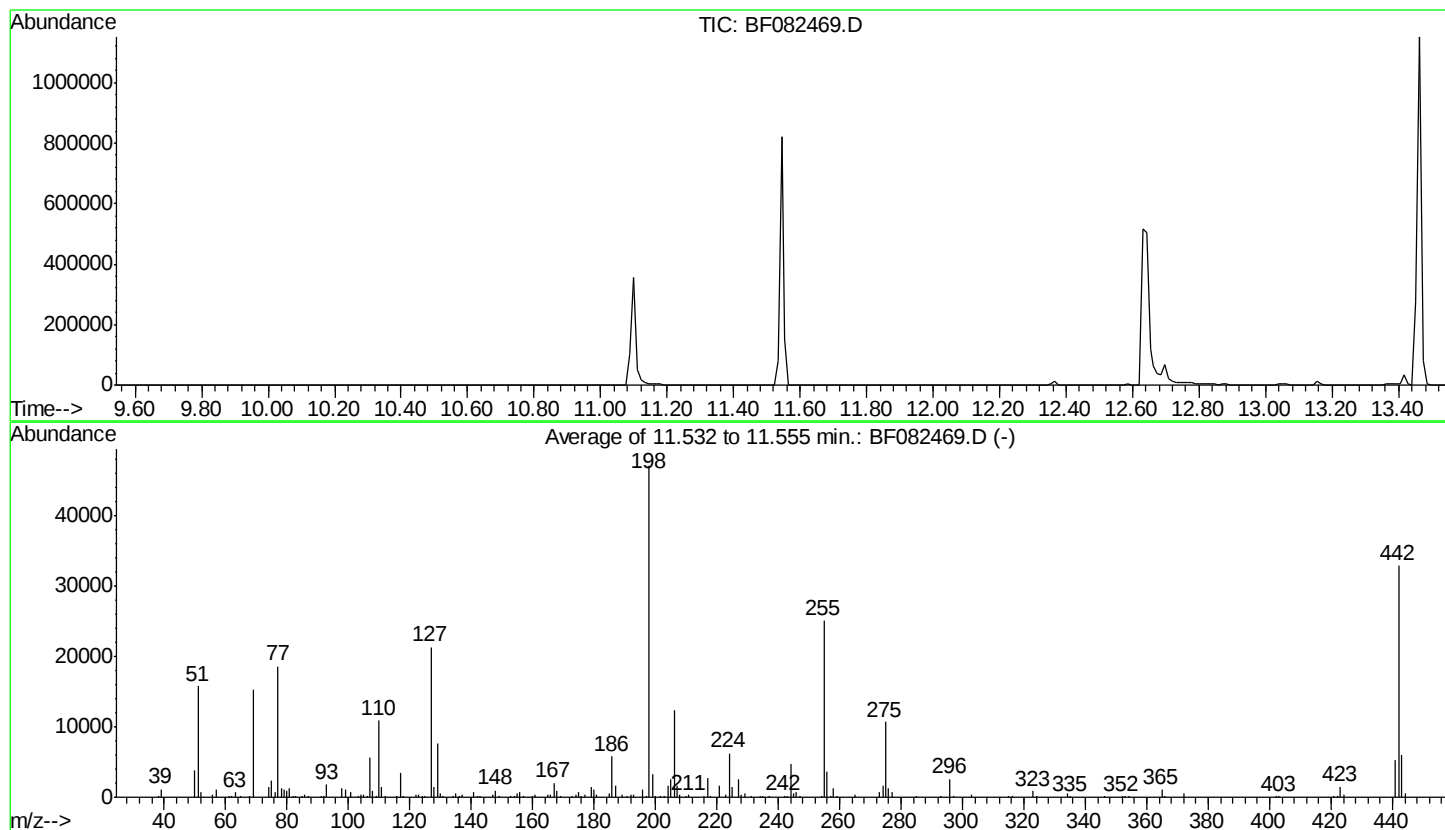

AutoFind: Scans 822, 823, 824; Background Corrected with Scan 819

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	33.4	15761	PASS
68	69	0.00	2	1.2	192	PASS
69	198	0.00	100	32.6	15380	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	45.3	21369	PASS
197	198	0.00	2	0.4	194	PASS
198	198	100	100	100.0	47179	PASS
199	198	5	9	6.8	3225	PASS
275	198	10	60	22.8	10738	PASS
365	198	1	100	2.2	1028	PASS
441	442	0.01	24	15.9	5252	PASS
442	198	50	100	69.8	32942	PASS
443	442	15	24	18.3	6019	PASS