
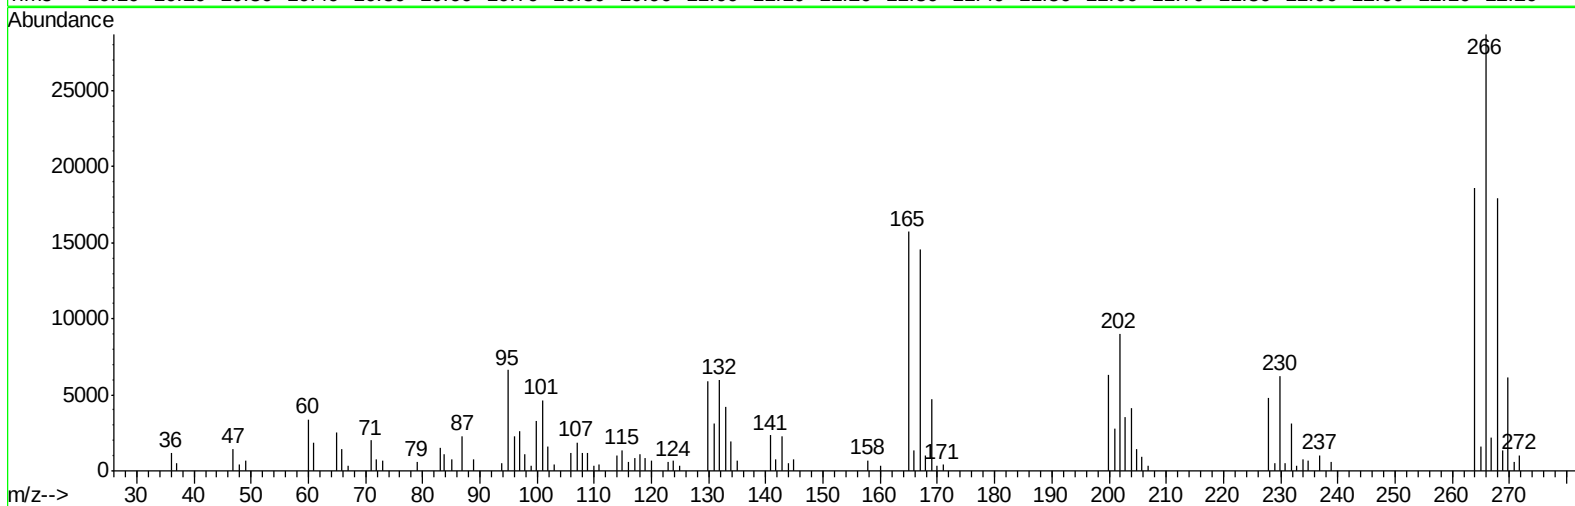


Data Path : Z:\HPCHEM1\BNA F\DATA\BF102317\
Data File : BF099760.D
Acq On : 23 Oct 2017 15:38
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 24 07:44:50 2017
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF102317.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Oct 23 23:39:26 2017
Response via : Initial Calibration

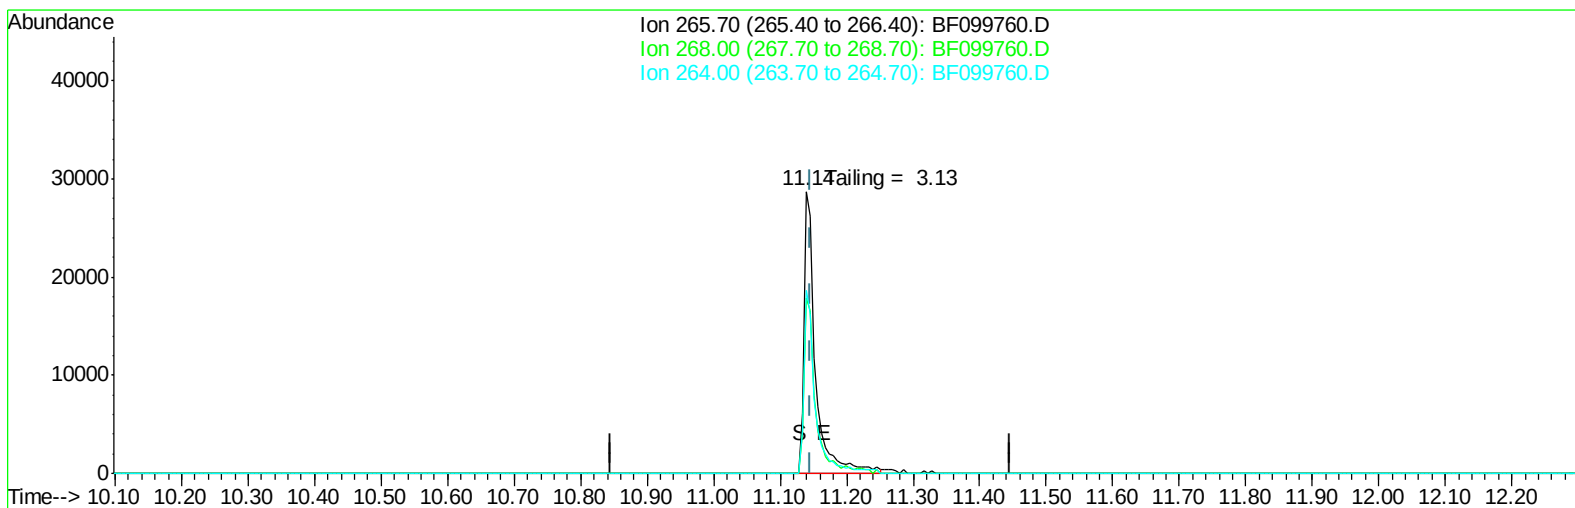

TIC: BF099760.D

(69) Pentachlorophenol (C)



11.139min (-0.006) 51919.13ng

response 35602

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	62.49
264.00	61.90	64.86
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA F\DATA\BF102317\
Data File : BF099760.D
Acq On : 23 Oct 2017 15:38
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 24 07:44:50 2017
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF102317.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Oct 23 23:39:26 2017
Response via : Initial Calibration

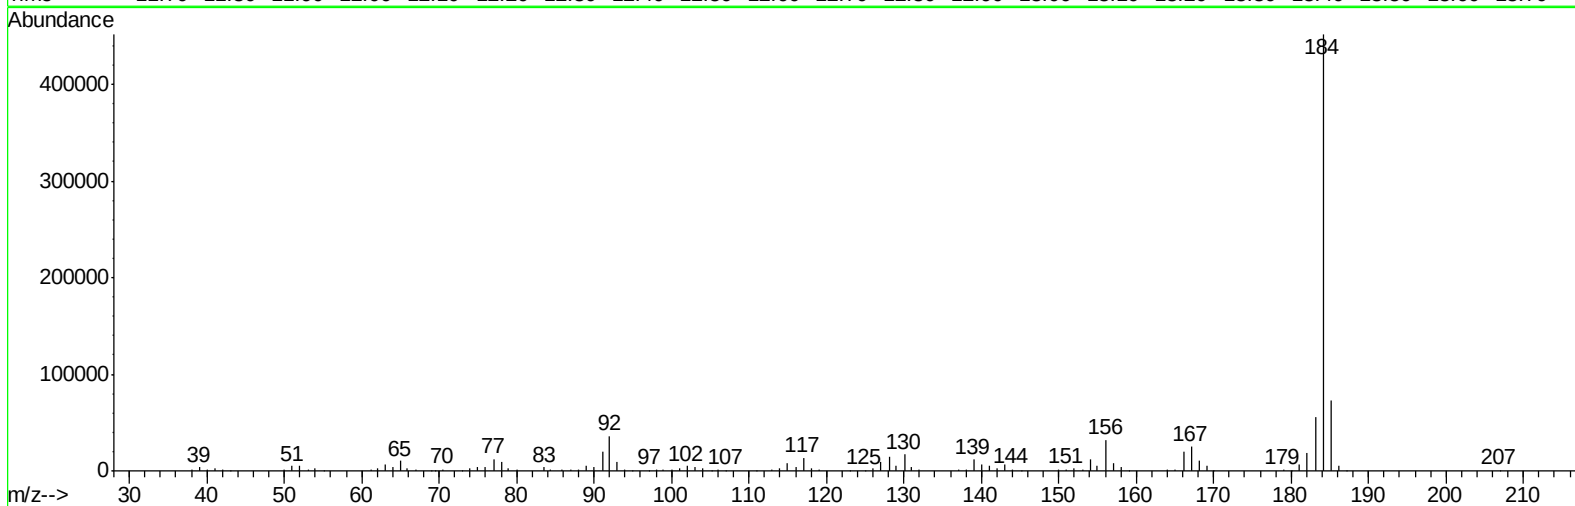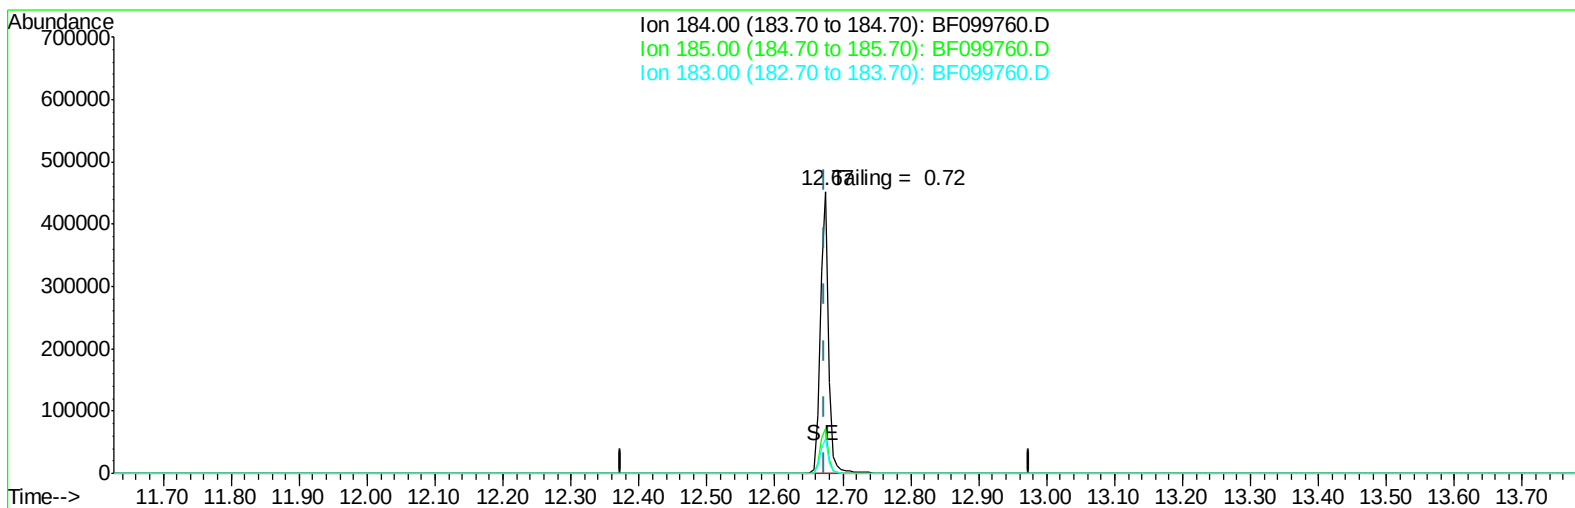

TIC: BF099760.D

(76) Benzidine

12.674min (-0.000) 0.00ng

response 384814

Ion	Exp%	Act%
184.00	100	100
185.00	15.70	16.07
183.00	11.60	12.20
0.00	0.00	0.00