


Data Path : Z:\HPCHEM1\BNA F\Data\BF102317\
 Data File : BF099751.D
 Acq On : 23 Oct 2017 10:35
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF102317.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Oct 23 23:39:26 2017

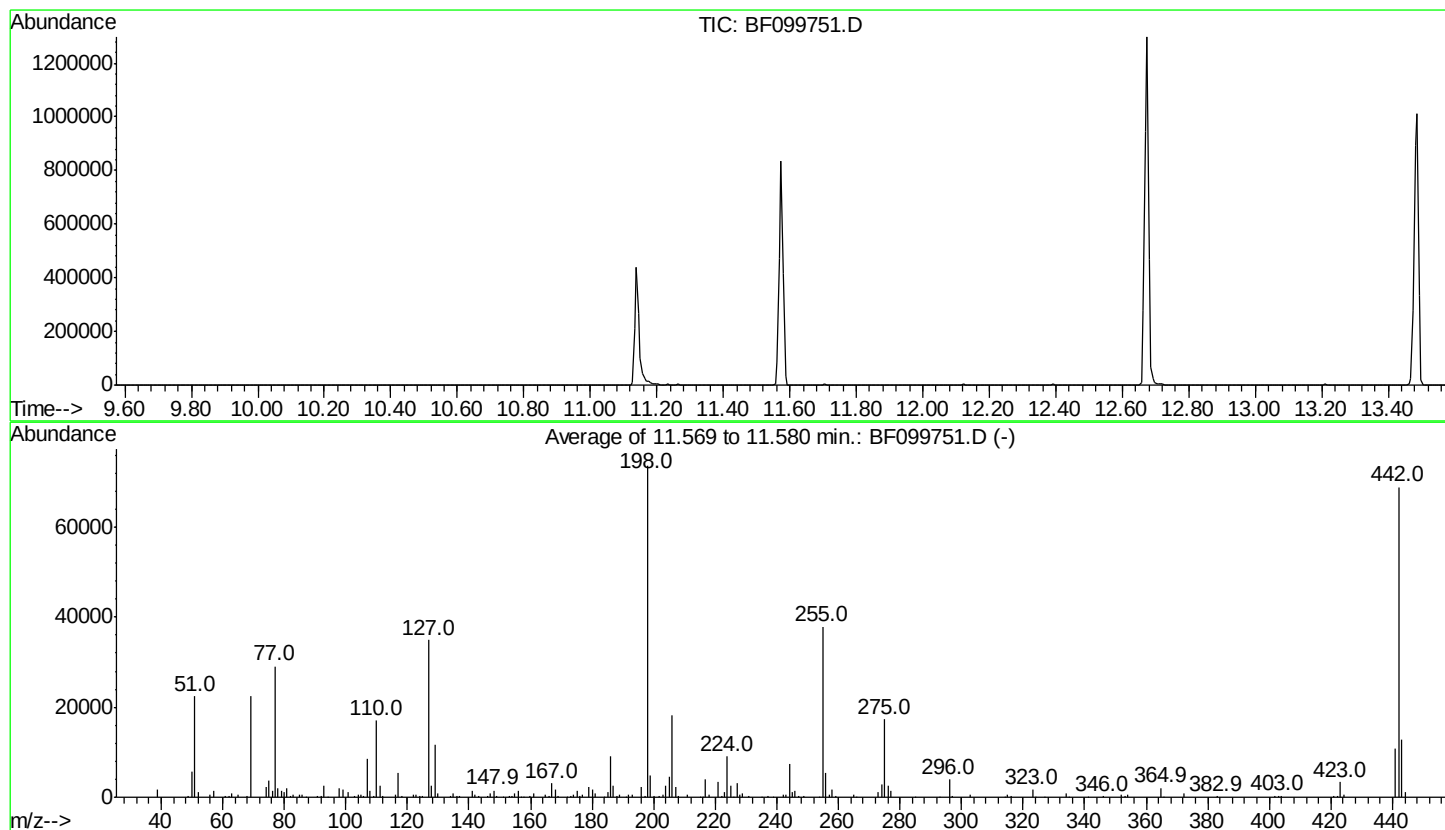

AutoFind: Scans 1612, 1613, 1614; Background Corrected with Scan 1607

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	30.4	22380	PASS
68	69	0.00	2	1.7	378	PASS
69	198	0.00	100	30.6	22514	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	47.3	34845	PASS
197	198	0.00	2	0.6	430	PASS
198	198	100	100	100.0	73650	PASS
199	198	5	9	6.6	4838	PASS
275	198	10	60	23.4	17232	PASS
365	198	1	100	2.8	2033	PASS
441	442	0.01	24	15.8	10871	PASS
442	198	50	100	93.6	68954	PASS
443	442	15	24	18.5	12727	PASS