


Data Path : Z:\HPCHEM1\BNA F\Data\BF102317\
 Data File : BF099760.D
 Acq On : 23 Oct 2017 15:38
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF102317.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Oct 23 23:39:26 2017

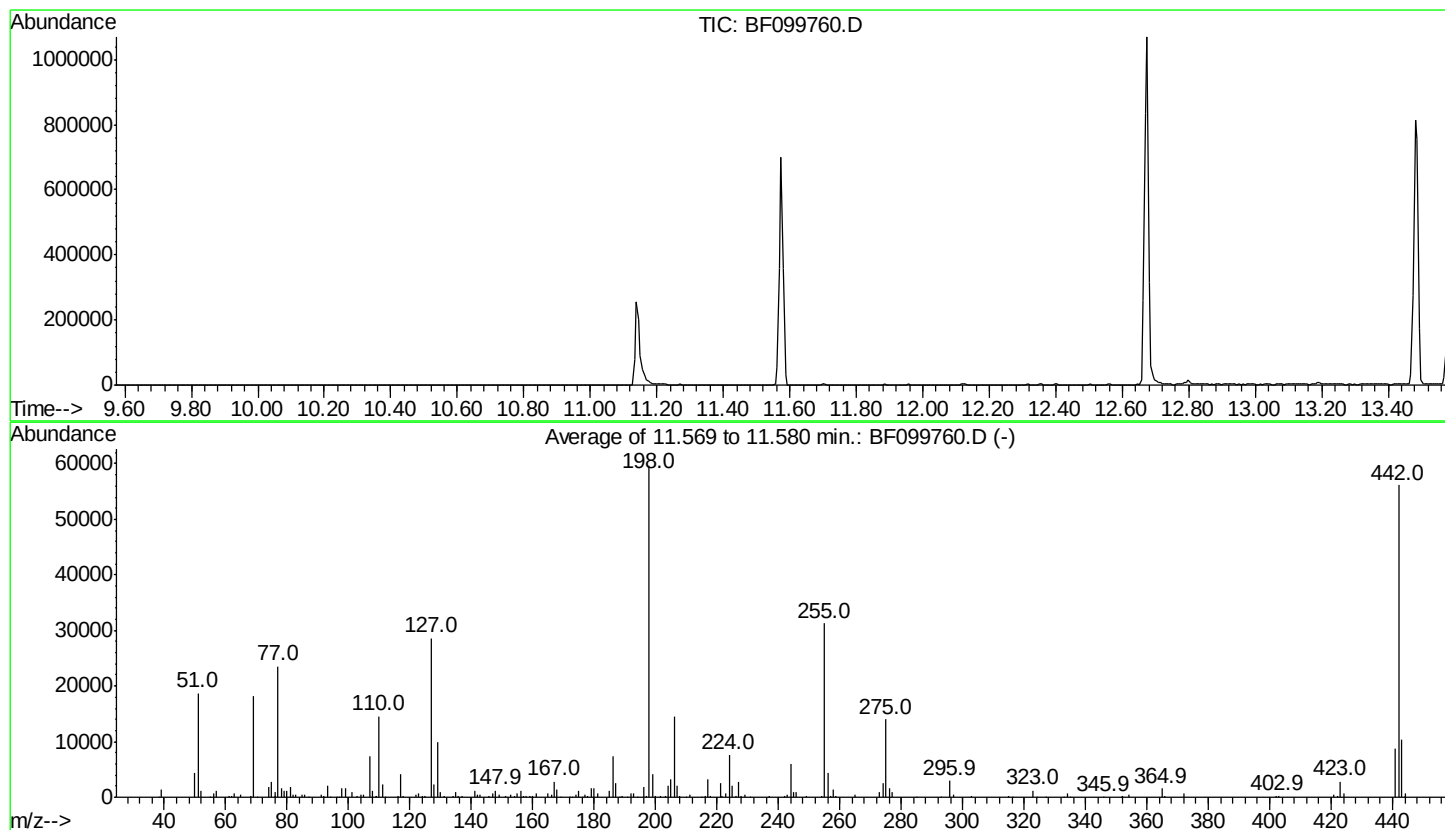

AutoFind: Scans 1612, 1613, 1614; Background Corrected with Scan 1607

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	31.4	18715	PASS
68	69	0.00	2	1.9	344	PASS
69	198	0.00	100	30.6	18235	PASS
70	69	0.00	2	0.6	106	PASS
127	198	10	80	48.0	28608	PASS
197	198	0.00	2	0.3	191	PASS
198	198	100	100	100.0	59653	PASS
199	198	5	9	6.9	4112	PASS
275	198	10	60	23.5	14000	PASS
365	198	1	100	2.6	1534	PASS
441	442	0.01	24	15.8	8867	PASS
442	198	50	100	94.1	56157	PASS
443	442	15	24	18.4	10325	PASS