
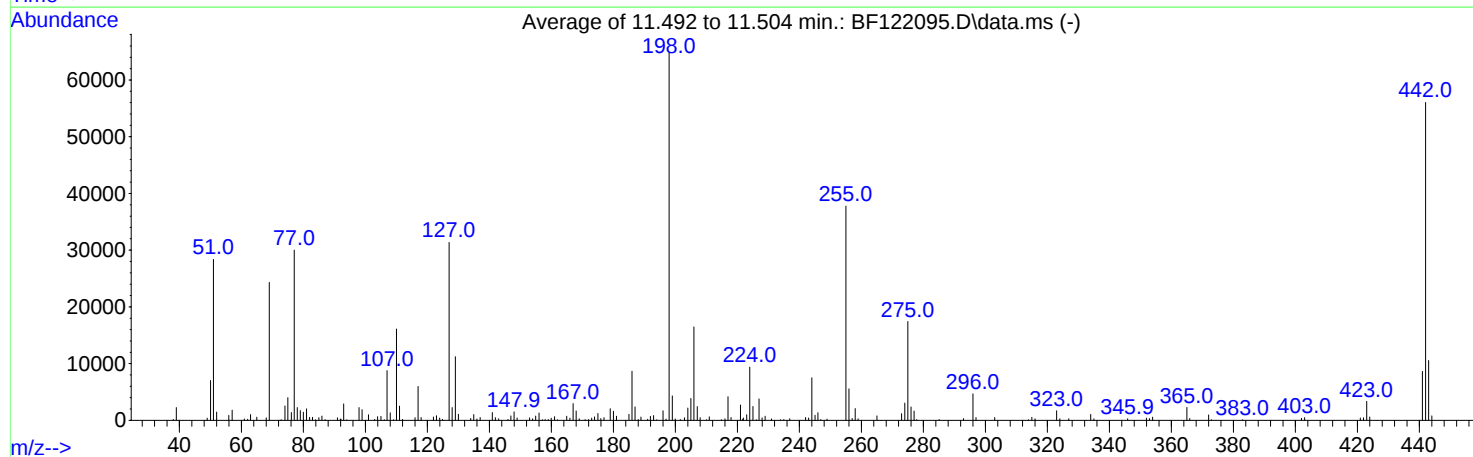


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF102320\
 Data File : BF122095.D
 Acq On : 23 Oct 2020 12:08
 Operator : JU/CG
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF101220.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Oct 21 12:04:42 2020

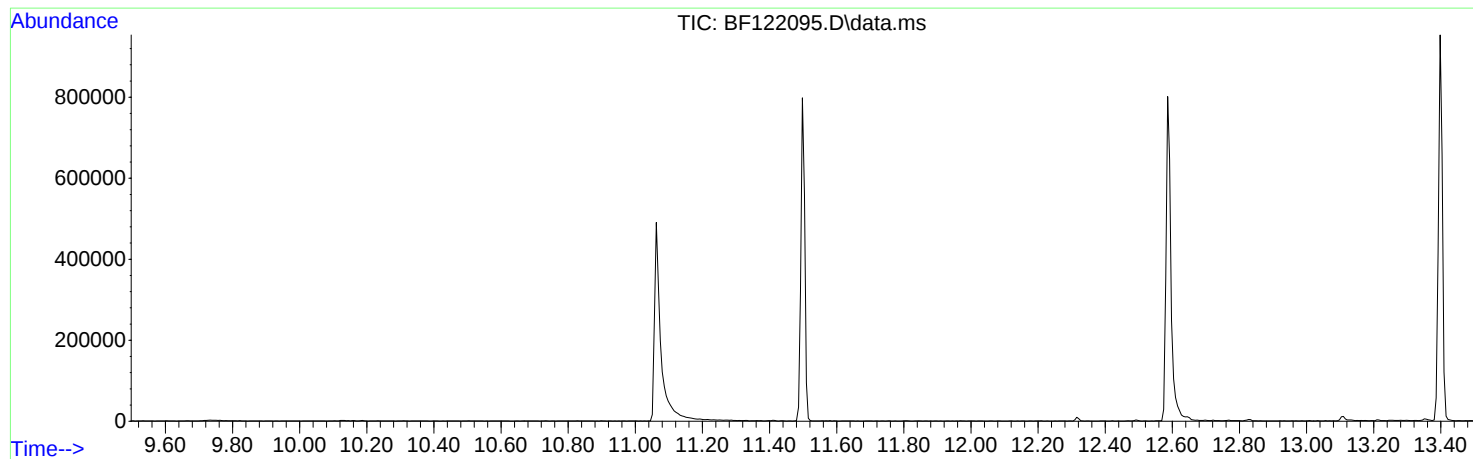

AutoFind: Scans 1599, 1600, 1601; Background Corrected with Scan 1594

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	43.8	28376	PASS
68	69	0.00	2	1.9	450	PASS
69	198	0.00	100	37.5	24320	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	48.4	31371	PASS
197	198	0.00	2	0.4	230	PASS
198	198	100	100	100.0	64840	PASS
199	198	5	9	6.6	4309	PASS
275	198	10	60	26.9	17418	PASS
365	198	1	100	3.5	2279	PASS
441	198	0.01	100	13.3	8646	PASS
442	198	50	100	86.5	56055	PASS
443	442	15	24	18.8	10549	PASS