
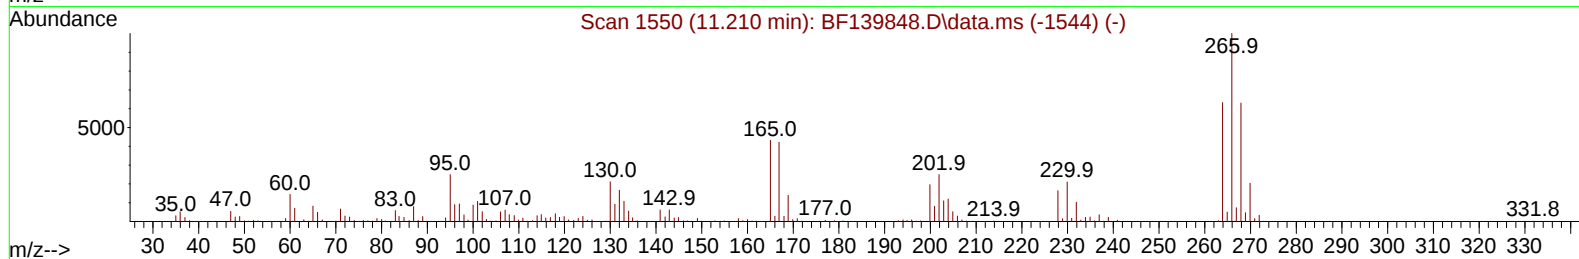
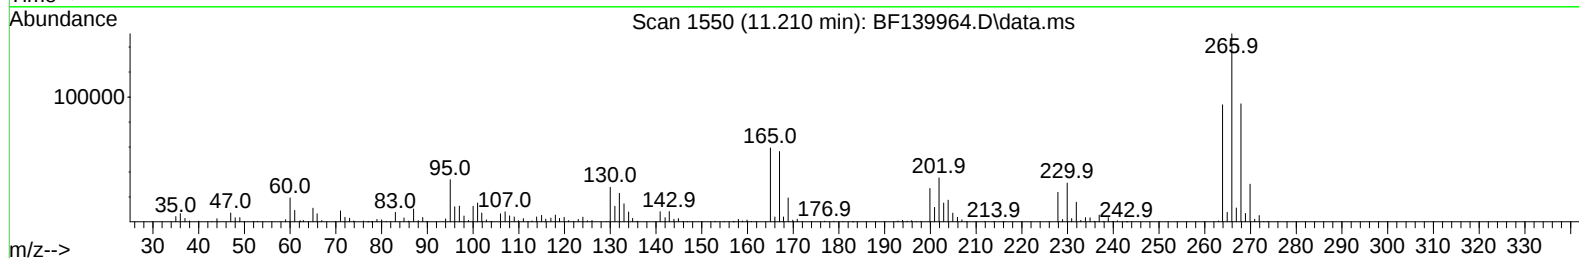


Data Path : Z:\svoasrv\HPCHEM1\BNA\_F\Data\BF102324\  
Data File : BF139964.D  
Acq On : 23 Oct 2024 15:01  
Operator : RC/JU  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 23 15:33:42 2024  
Quant Method : Z:\svoasrv\HPCHEM1\BNA\_F\Methods\8270-BF101824.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Fri Oct 18 15:07:50 2024  
Response via : Initial Calibration

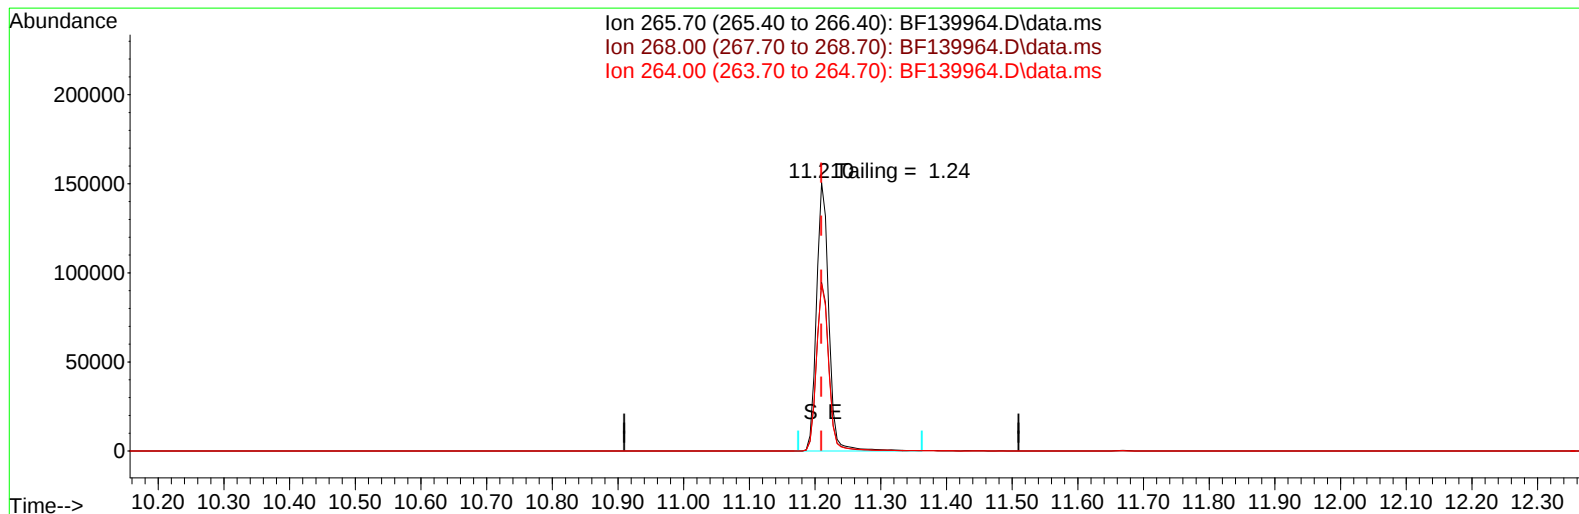

TIC: BF139964.D\data.ms

**(70) Pentachlorophenol (C)**




**11.210min (+ 0.000) 37980.39 ng**

**response 197630**

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 265.70 | 100.00 | 100.00 |
| 268.00 | 63.00  | 62.75  |
| 264.00 | 63.20  | 62.27  |
| 0.00   | 0.00   | 0.00   |

Data Path : Z:\svoasrv\HPCHEM1\BNA\_F\Data\BF102324\  
Data File : BF139964.D  
Acq On : 23 Oct 2024 15:01  
Operator : RC/JU  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 23 15:33:42 2024  
Quant Method : Z:\svoasrv\HPCHEM1\BNA\_F\Methods\8270-BF101824.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Fri Oct 18 15:07:50 2024  
Response via : Initial Calibration

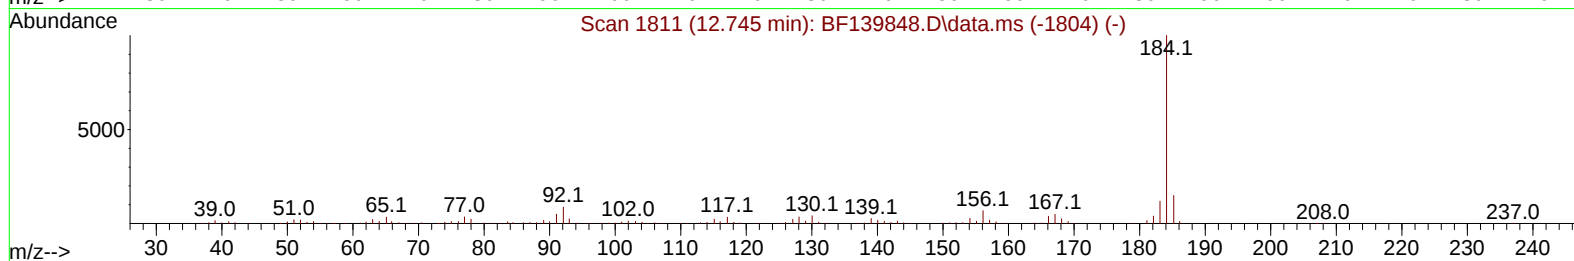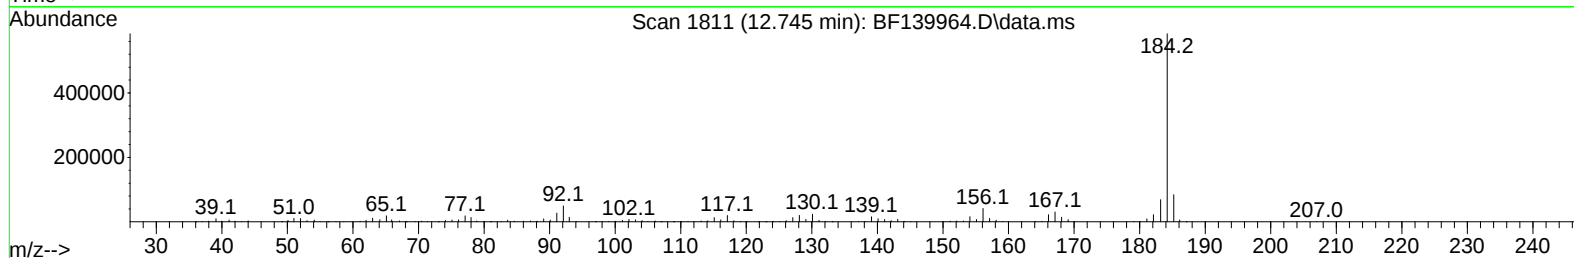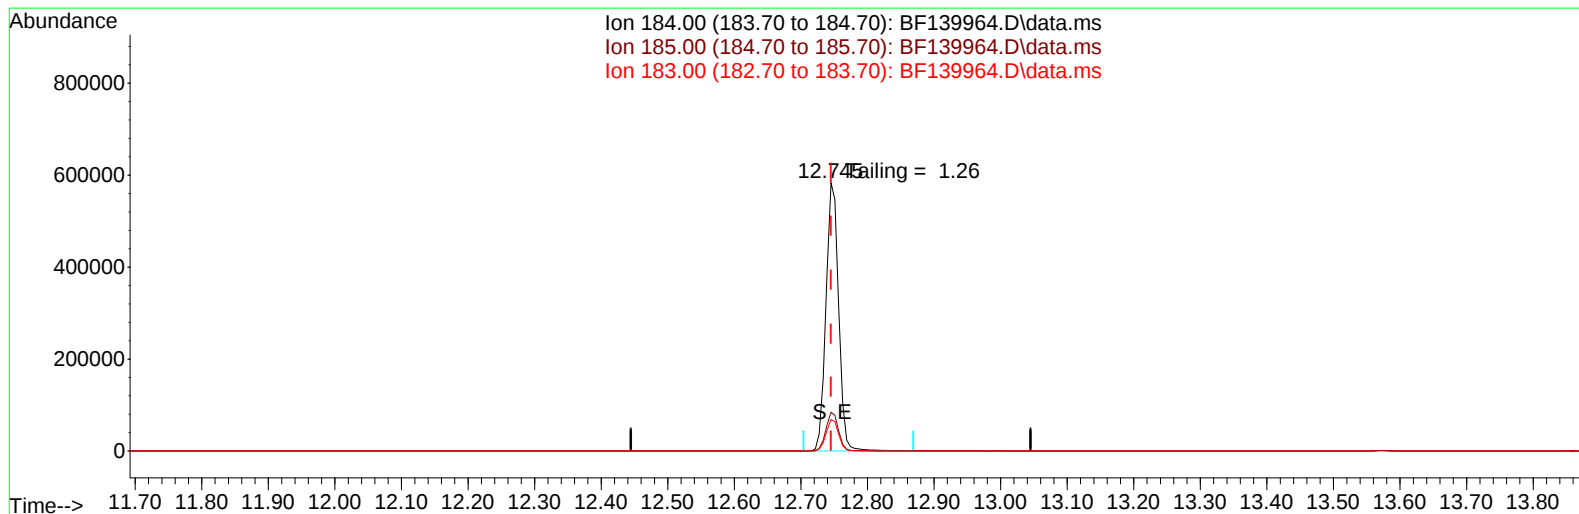

TIC: BF139964.D\data.ms

**(77) Benzidine**

12.745min (+ 0.000) 0.00 ng

response 775484

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 184.00 | 100.00 | 100.00 |
| 185.00 | 15.00  | 14.45  |
| 183.00 | 11.80  | 11.75  |
| 0.00   | 0.00   | 0.00   |