
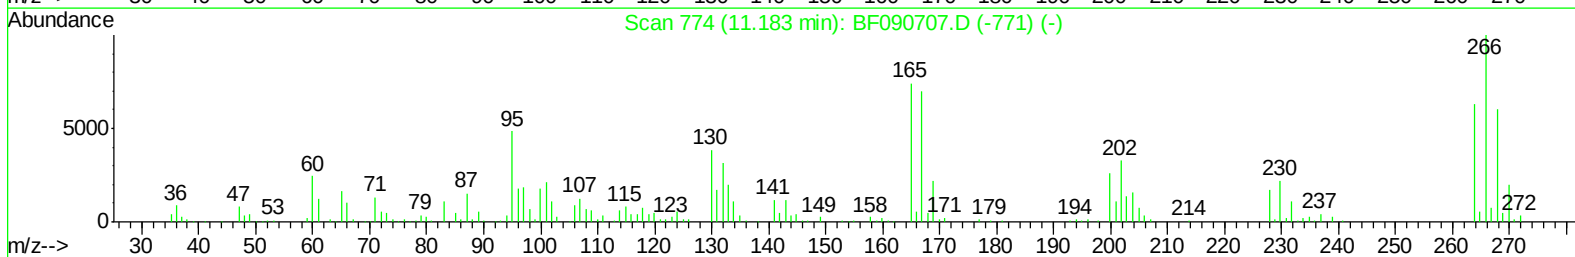
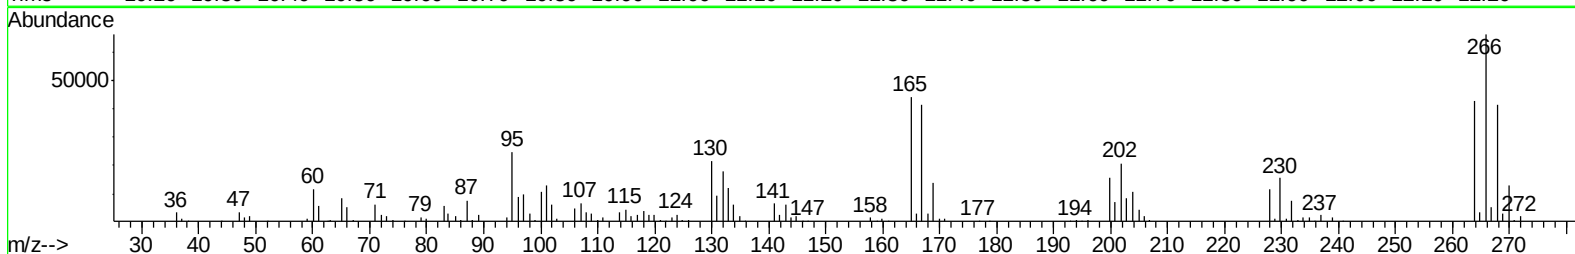


Data Path : Z:\HPCHEM1\BNA\_F\DATA\BF102416\  
Data File : BF090787.D  
Acq On : 24 Oct 2016 13:37  
Operator : UM/SJ  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 25 01:34:05 2016  
Quant Method : Z:\HPCHEM1\BNA\_F\METHODS\8270-BF102116.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Fri Oct 21 17:36:31 2016  
Response via : Initial Calibration

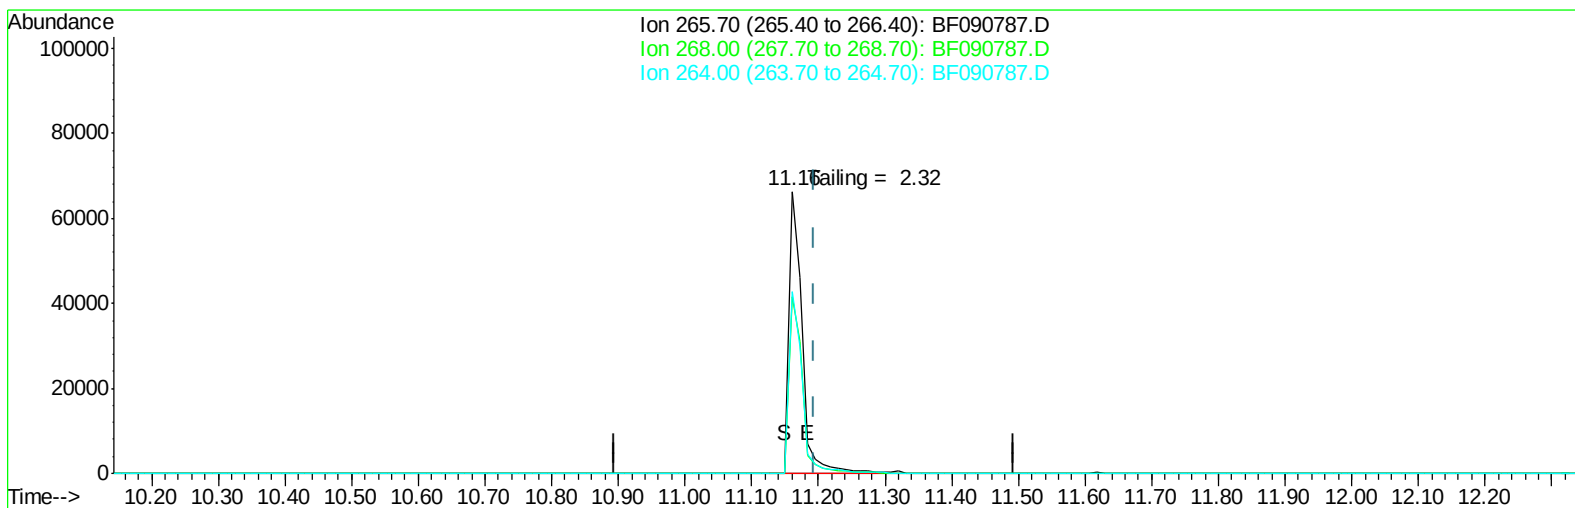

TIC: BF090787.D

(69) Pentachlorophenol (C)




11.161min (-0.033) 3021.08ng

response 90331

| Ion    | Exp%  | Act%  |
|--------|-------|-------|
| 265.70 | 100   | 100   |
| 268.00 | 62.20 | 62.61 |
| 264.00 | 62.70 | 64.46 |
| 0.00   | 0.00  | 0.00  |

Data Path : Z:\HPCHEM1\BNA\_F\DATA\BF102416\  
 Data File : BF090787.D  
 Acq On : 24 Oct 2016 13:37  
 Operator : UM/SJ  
 Sample : DFTPP  
 Misc :  
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 25 01:34:05 2016  
 Quant Method : Z:\HPCHEM1\BNA\_F\METHODS\8270-BF102116.M  
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 QLast Update : Fri Oct 21 17:36:31 2016  
 Response via : Initial Calibration

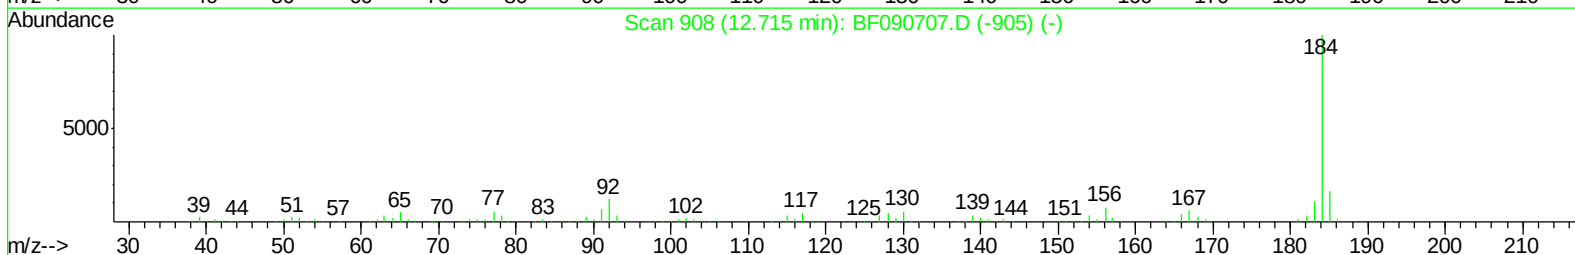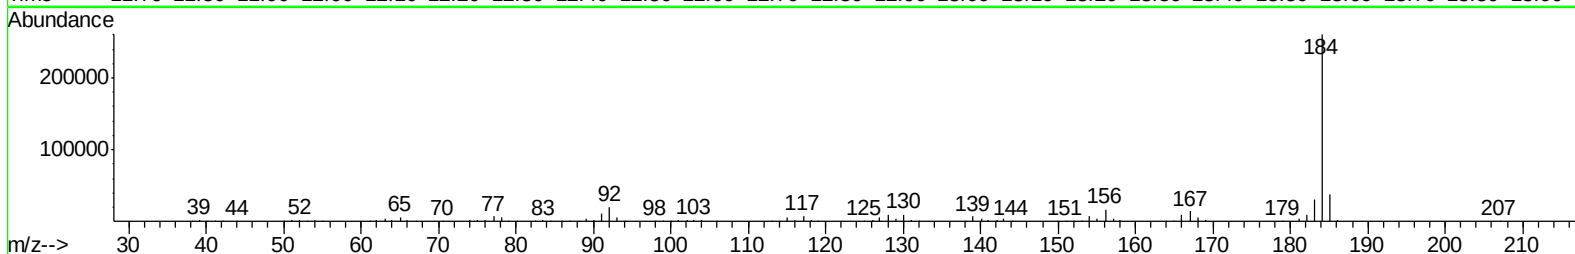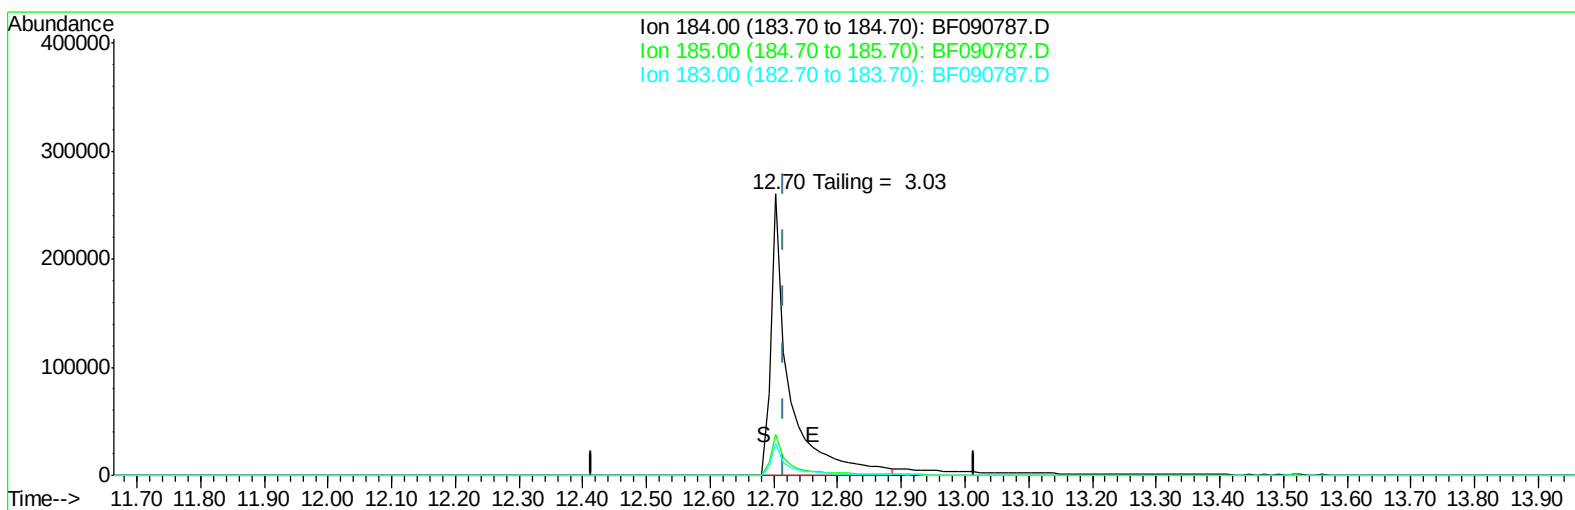

TIC: BF090787.D

(76) Benzidine

12.704min (-0.011) 0.00ng

response 540760

| Ion    | Exp%  | Act%   |
|--------|-------|--------|
| 184.00 | 100   | 100    |
| 185.00 | 14.70 | 14.63  |
| 183.00 | 9.50  | 11.51# |
| 0.00   | 0.00  | 0.00   |