

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF102416\
 Data File : BF090795.D
 Acq On : 24 Oct 2016 18:47
 Operator : UM/SJ
 Sample : H5366-01
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 FK-EF-01-002-ABCD

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF102116.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.011	232	234	247	rBV	612527	1034952	19.21%	2.318%
2	5.434	269	271	274	rBV	3276754	4273194	79.32%	9.569%
3	6.474	359	362	364	rBV	3803697	4704831	87.33%	10.536%
4	6.600	370	373	376	rBV	4387283	4496246	83.46%	10.068%
5	6.829	391	393	404	rBV	884503	1177398	21.86%	2.637%
6	6.989	404	407	409	rBV	3976201	3713701	68.93%	8.316%
7	7.400	440	443	445	rBV	2540797	2845082	52.81%	6.371%
8	8.120	503	506	508	rBV	1577177	1608089	29.85%	3.601%
9	9.195	597	600	603	rBV	4987485	5387291	100.00%	12.064%
10	9.595	632	635	637	rBV	786471	843382	15.66%	1.889%
11	9.869	657	659	662	rBV	1943726	1867204	34.66%	4.181%
12	10.315	694	698	699	rBV	59305	89581	1.66%	0.201%
13	10.532	714	717	720	rBV	33979	59165	1.10%	0.132%
14	10.658	726	728	731	rBV2	2434043	3210426	59.59%	7.189%
15	10.783	737	739	744	rVB	113932	142746	2.65%	0.320%
16	11.229	776	778	780	rBV	61615	60757	1.13%	0.136%
17	11.355	787	789	801	rBV	1768141	1764476	32.75%	3.951%
18	12.944	926	928	931	rBV	4458130	4911484	91.17%	10.998%
19	13.847	1005	1007	1013	rBV	55245	100209	1.86%	0.224%
20	13.995	1017	1020	1028	rBV	1272158	1372186	25.47%	3.073%
21	15.424	1142	1145	1155	rVB	740195	994456	18.46%	2.227%


Sum of corrected areas: 44656856

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF102416\
Data File : BF090795.D
Acq On : 24 Oct 2016 18:47
Operator : UM/SJ
Sample : H5366-01
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
FK-EF-01-002-ABCD

Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF102116.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

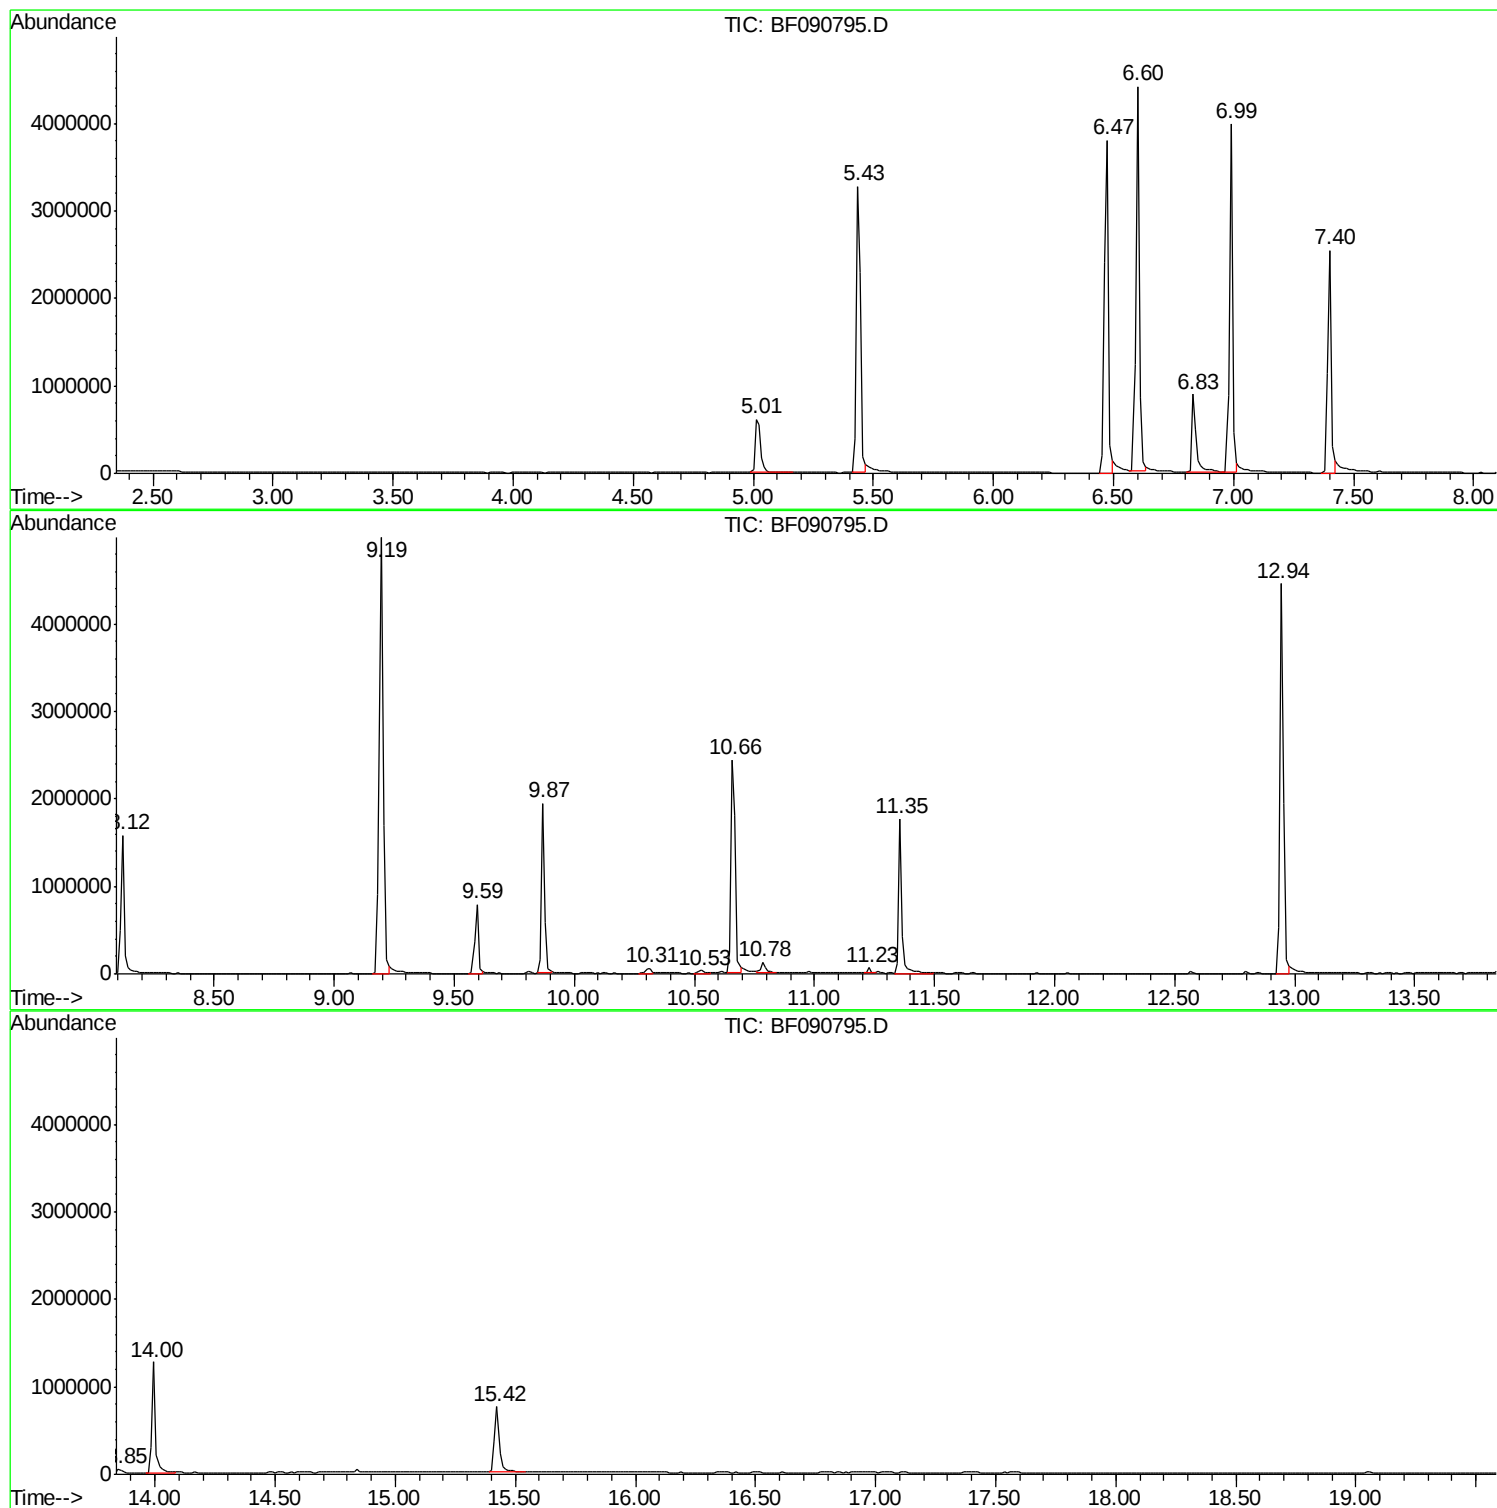

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF102416\
Data File : BF090795.D
Acq On : 24 Oct 2016 18:47
Operator : UM/SJ
Sample : H5366-01
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
FK-EF-01-002-ABCD










Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF102116.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 2-Pentanone, 4-hydroxy-4-me... Concentration Rank 3

R.T.	EstConc	Area	Relative to ISTD	R.T.
5.01	17.58 ng	1034950	1,4-Dichlorobenzene-d4	6.83

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			2-Pentanone, 4-hydroxy-4-methyl-	116	C6H12O2	000123-42-2	59
2			Propane, 2-methyl-2-(1-methyleth...	116	C7H16O	017348-59-3	33
3			Acetic acid, cyano-, 1,1-dimethyl...	141	C7H11NO2	001116-98-9	25
4			1-Propen-2-ol, acetate	100	C5H8O2	000108-22-5	10
5			Morpholine, 4-methyl-	101	C5H11NO	000109-02-4	9

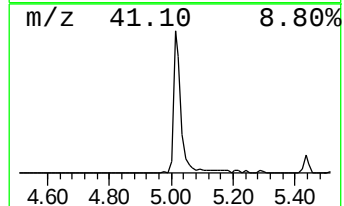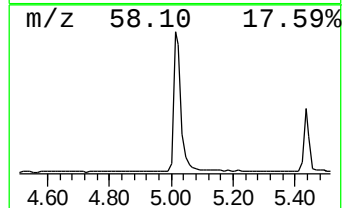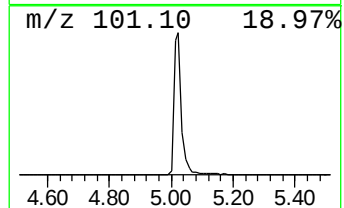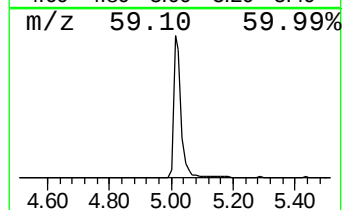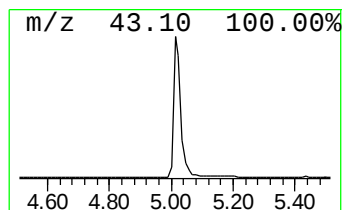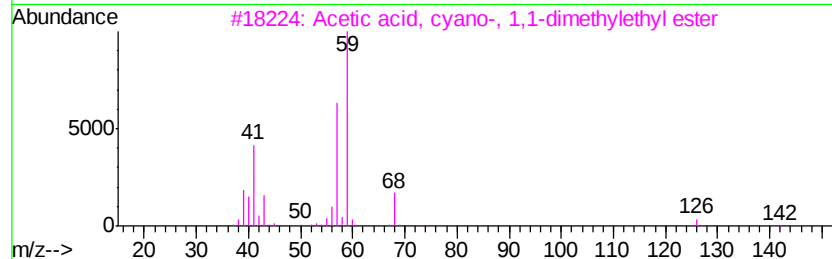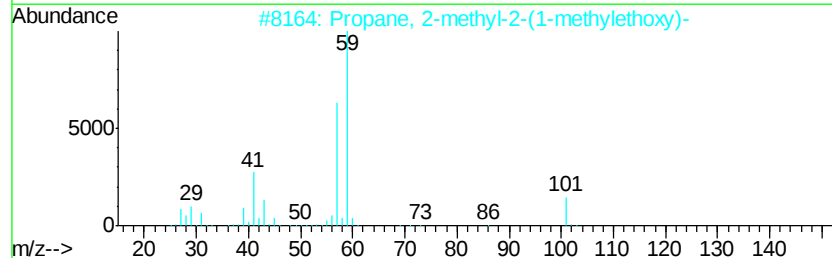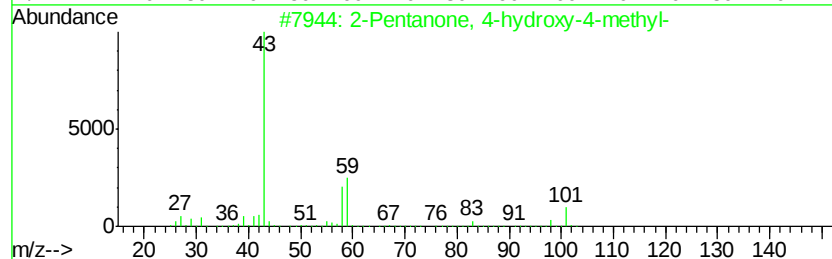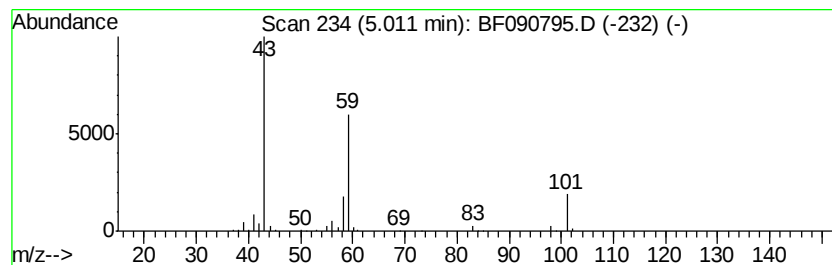

Data Path : Z:\HPCHEM1\BNA F\DATA\BF102416\
Data File : BF090795.D
Acq On : 24 Oct 2016 18:47
Operator : UM/SJ
Sample : H5366-01
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
FK-EF-01-002-ABCD










Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF102116.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

Peak Number 2 unknown6.60 Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
6.60	76.38 ng	4496250	1,4-Dichlorobenzene-d4	6.83

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	(E)-3-Chloro-2-methyl-2-pentenal	132	C6H9ClO	031357-76-3	17
2		3-Chloro-6-fluoro-pyrazine	132	C4H2ClFN2	1000146-10-7	16
3		5-Aminoindole	132	C8H8N2	005192-03-0	12
4		5-Fluoro-2-chloropyrimidine	132	C4H2ClFN2	062802-42-0	9
5		4-Chloro-6-fluoro-pyrimidine	132	C4H2ClFN2	051422-01-6	9

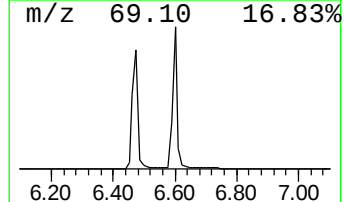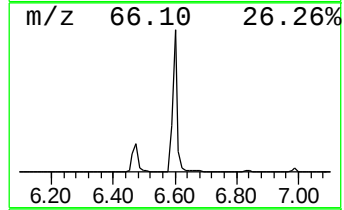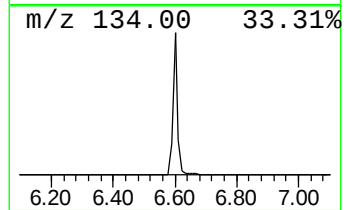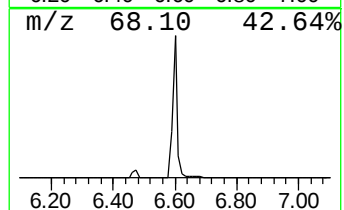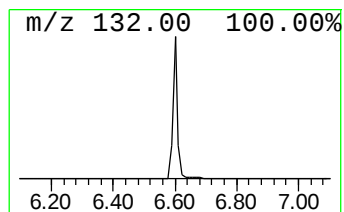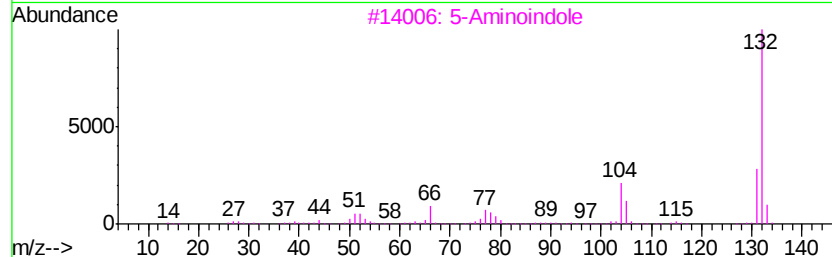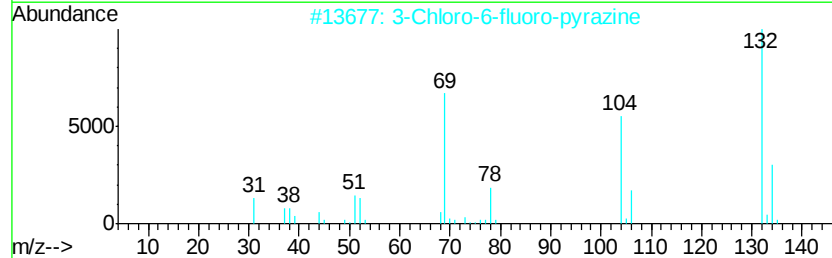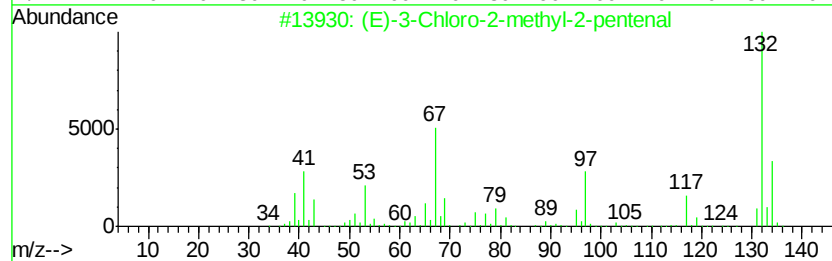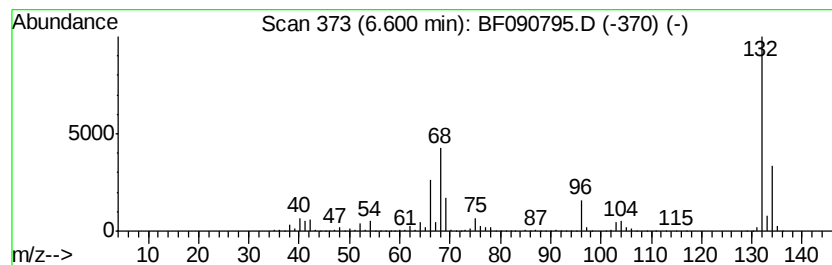

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF102416\
Data File : BF090795.D
Acq On : 24 Oct 2016 18:47
Operator : UM/SJ
Sample : H5366-01
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
FK-EF-01-002-ABCD

Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF102116.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
2-Pentanone, 4-hy...	5.01	17.6	ng	1034950	1	6.83	1177400	20.0
unknown6.60	6.60	76.4	ng	4496250	1	6.83	1177400	20.0