


Data Path : Z:\HPCHEM1\BNA F\Data\BF102417\
 Data File : BF099782.D
 Acq On : 24 Oct 2017 12:15
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF102317.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Oct 23 23:39:26 2017

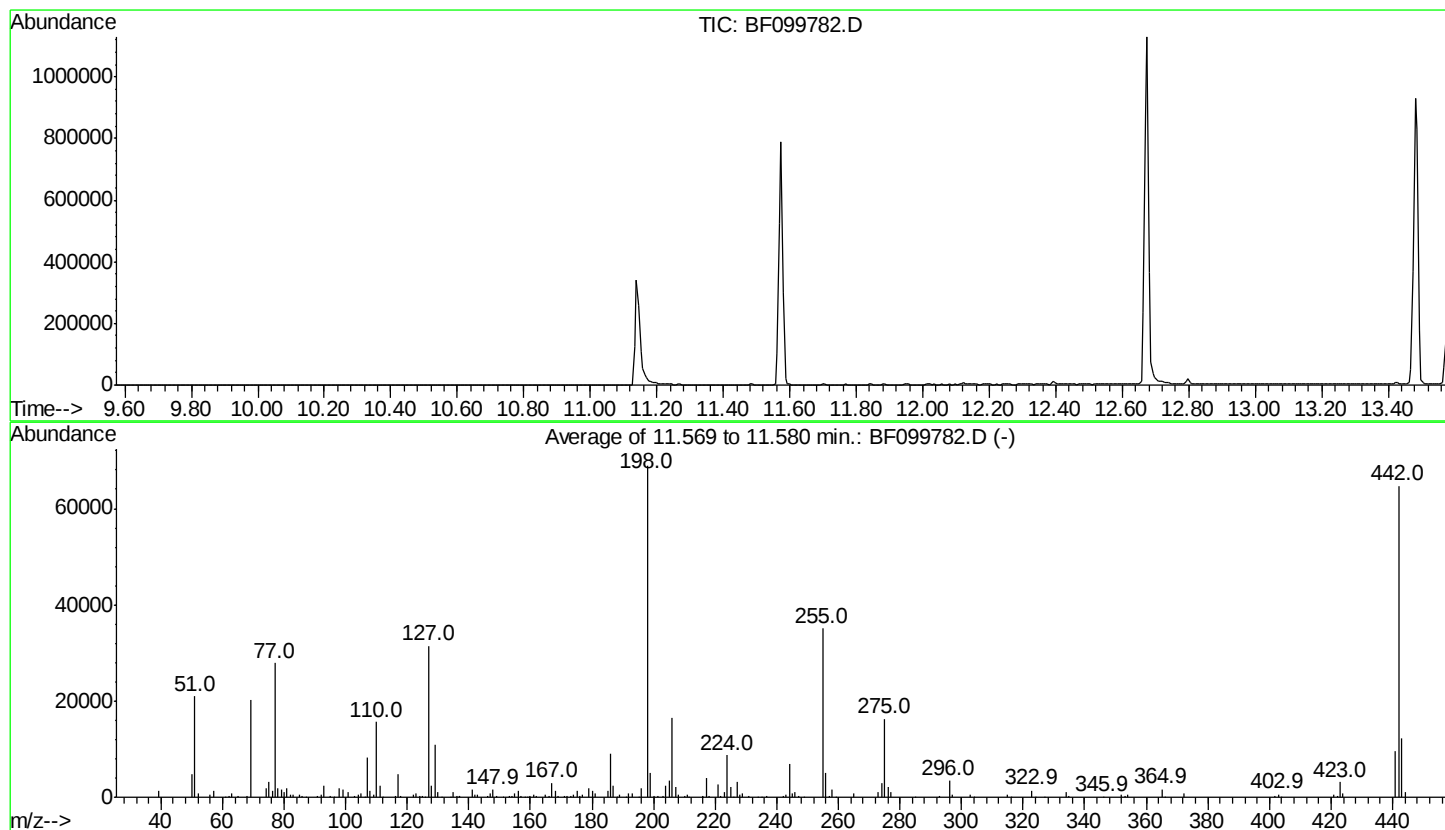

AutoFind: Scans 1612, 1613, 1614; Background Corrected with Scan 1607

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	30.5	20997	PASS
68	69	0.00	2	1.7	347	PASS
69	198	0.00	100	29.2	20127	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	45.7	31485	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	68928	PASS
199	198	5	9	7.2	4948	PASS
275	198	10	60	23.6	16264	PASS
365	198	1	100	2.4	1682	PASS
441	442	0.01	24	14.9	9657	PASS
442	198	50	100	93.9	64698	PASS
443	442	15	24	19.0	12270	PASS