

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF102419\
 Data File : BF117531.D
 Acq On : 25 Oct 2019 00:39
 Operator : JU
 Sample : K5498-07 5X
 Misc :
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 196-00-(0-1)

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0
 Filtering: 5
 Min Area: 3 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF101819.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.363	554	557	575	rBV	93566	141897	36.64%	4.335%
2	6.393	729	732	749	rBV	113490	178452	46.08%	5.451%
3	6.510	749	752	766	rVB	159715	189553	48.95%	5.790%
4	6.734	787	790	807	rBV	304551	270504	69.85%	8.263%
5	6.892	813	817	825	rBV	135722	129901	33.54%	3.968%
6	7.304	884	887	898	rBV	57754	86416	22.31%	2.640%
7	8.016	1005	1008	1017	rBV	421743	359312	92.78%	10.976%
8	9.086	1187	1190	1201	rBV	191642	169799	43.85%	5.187%
9	9.486	1255	1258	1265	rVB	18282	16542	4.27%	0.505%
10	9.769	1302	1306	1319	rBV	447010	387267	100.00%	11.830%
11	10.563	1438	1441	1450	rVB	67879	69645	17.98%	2.127%
12	10.686	1456	1462	1465	rBV3	6525	8805	2.27%	0.269%
13	11.145	1537	1540	1544	rVB3	5904	6306	1.63%	0.193%
14	11.257	1555	1559	1562	rBV	318943	294706	76.10%	9.003%
15	11.763	1639	1645	1647	rBV3	3889	4700	1.21%	0.144%
16	11.786	1647	1649	1655	rVB6	5566	7106	1.83%	0.217%
17	11.869	1660	1663	1666	rBV2	9416	9626	2.49%	0.294%
18	12.233	1722	1725	1728	rBV5	4129	5577	1.44%	0.170%
19	12.310	1733	1738	1740	rBV2	5984	7978	2.06%	0.244%
20	12.339	1740	1743	1746	rBV4	5397	7636	1.97%	0.233%
21	12.469	1762	1765	1770	rBV	48235	46428	11.99%	1.418%
22	12.698	1798	1804	1811	rBV	63221	75261	19.43%	2.299%
23	12.763	1811	1815	1819	rVV7	4585	7960	2.06%	0.243%
24	12.833	1824	1827	1838	rVB	142940	138005	35.64%	4.216%
25	12.921	1838	1842	1843	rBV3	9982	11418	2.95%	0.349%
26	12.969	1847	1850	1853	rVB5	4466	5372	1.39%	0.164%
27	13.033	1853	1861	1863	rBV6	13520	27359	7.06%	0.836%
28	13.063	1863	1866	1868	rBV3	7590	8154	2.11%	0.249%
29	13.092	1869	1871	1875	rBV3	5991	6159	1.59%	0.188%
30	13.133	1875	1878	1879	rBV3	7143	6467	1.67%	0.198%
31	13.192	1886	1888	1889	rBV2	6830	4354	1.12%	0.133%
32	13.227	1892	1894	1897	rVB4	6930	7594	1.96%	0.232%
33	13.257	1897	1899	1900	rBV2	11713	8618	2.23%	0.263%
34	13.339	1911	1913	1916	rBV4	4783	4714	1.22%	0.144%

Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF102419\
Data File : BF117531.D
Acq On : 25 Oct 2019 00:39
Operator : JU
Sample : K5498-07 5X
Misc :
ALS Vial : 25 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
196-00-(0-1)

Integration Parameters: rteint.p
Integrator: RTE
Smoothing : ON Filtering: 5
Sampling : 1 Min Area: 3 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF101819.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

35	13.404	1922	1924	1927	rBV4	13217	12811	3.31%	0.391%
36	13.704	1973	1975	1976	rBV2	11416	9149	2.36%	0.279%
37	13.898	2004	2008	2012	rBV	276033	308307	79.61%	9.418%
38	15.333	2248	2252	2261	rVB	153980	233724	60.35%	7.140%


Sum of corrected areas: 3273582

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF102419\
Data File : BF117531.D
Acq On : 25 Oct 2019 00:39
Operator : JU
Sample : K5498-07 5X
Misc :
ALS Vial : 25 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
196-00-(0-1)

Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF101819.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

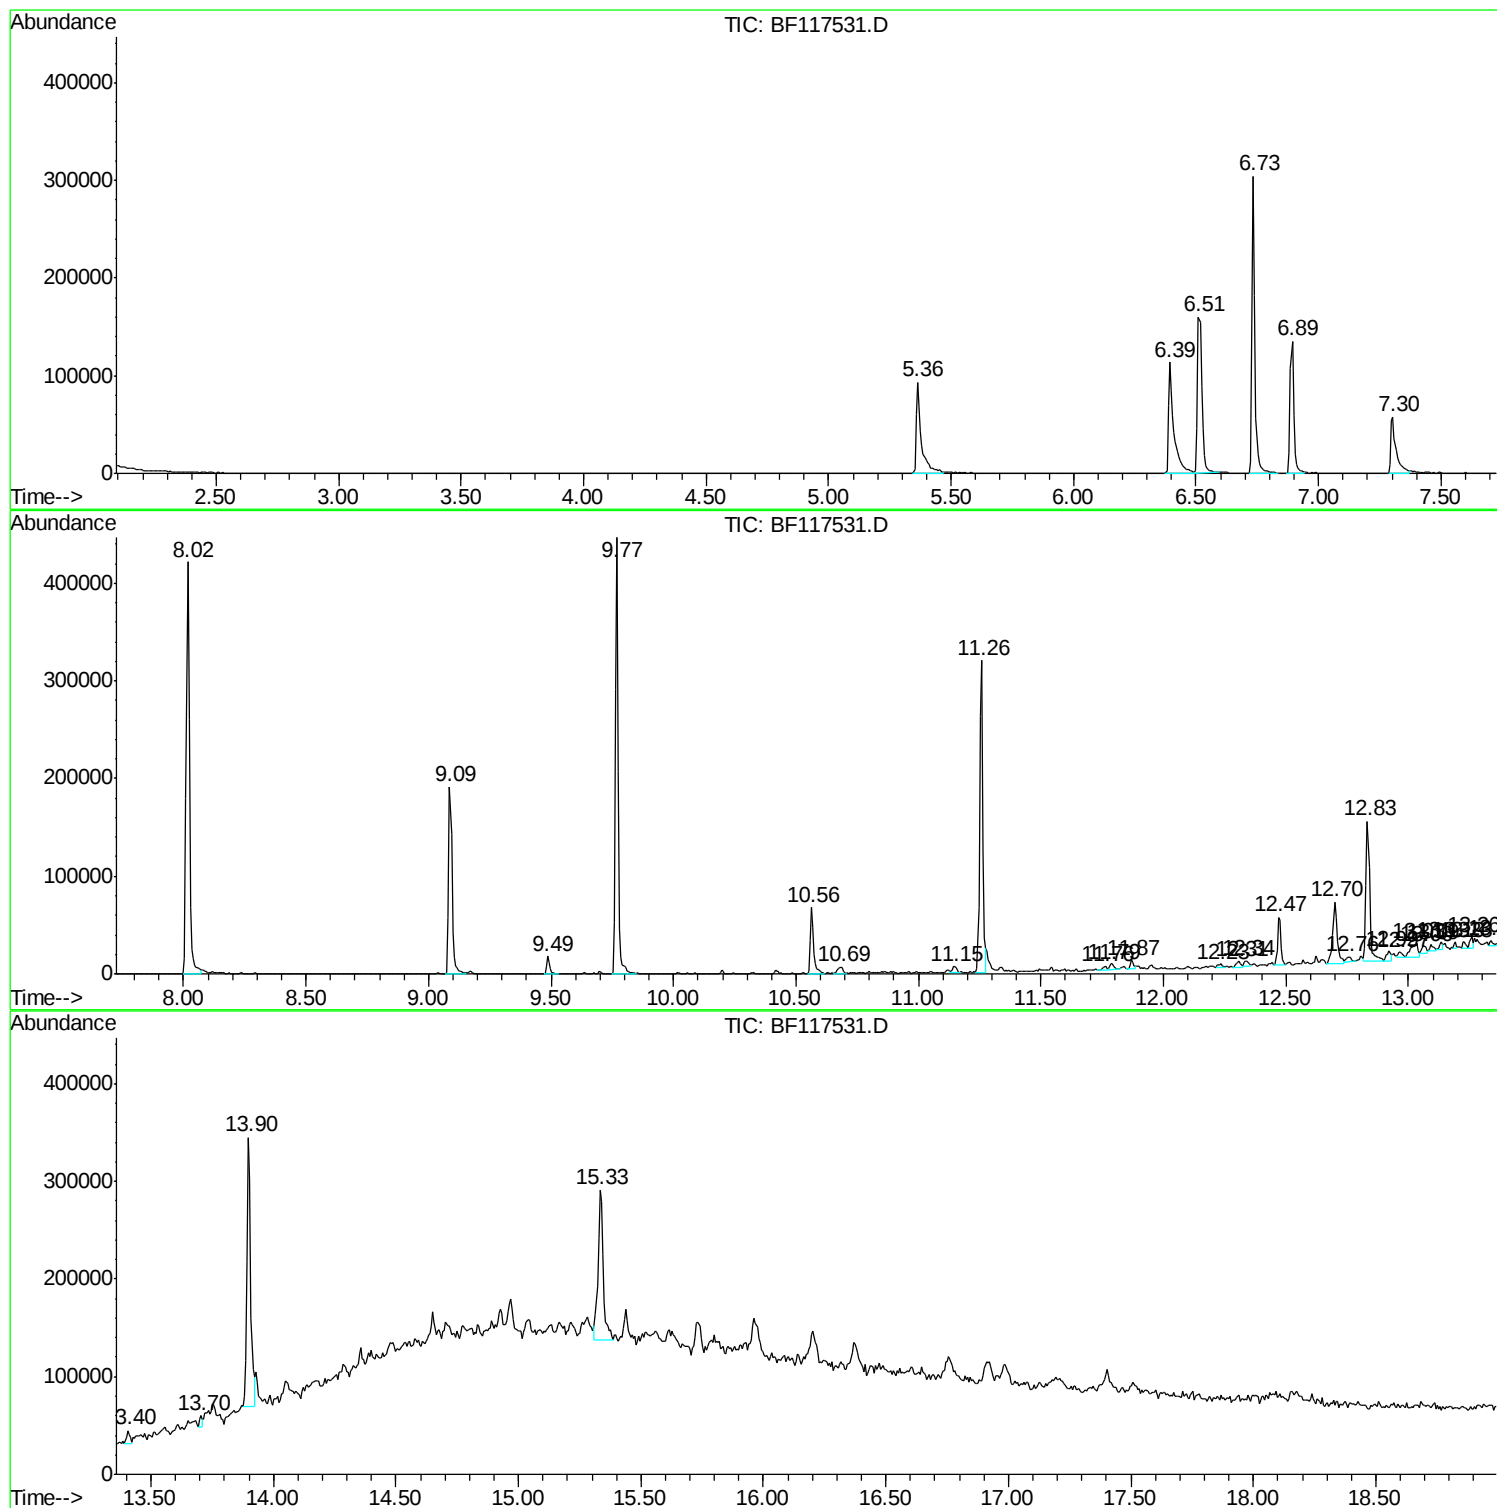

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF102419\
Data File : BF117531.D
Acq On : 25 Oct 2019 00:39
Operator : JU
Sample : K5498-07 5X
Misc :
ALS Vial : 25 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
196-00-(0-1)










Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF101819.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 unknown6.51 Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
6.51	14.01 ng	189553	1,4-Dichlorobenzene-d4	6.73

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	5-Aminoindole	132	C8H8N2	005192-03-0	22
2		3-Chloro-6-fluoro-pyrazine	132	C4H2ClFN2	1000146-10-7	16
3		1-Aminoindan	133	C9H11N	034698-41-4	9
4		Xenon	132	Xe	007440-63-3	9
5		2H-Cyclopenta[d]pyridazine, 2-me...	132	C8H8N2	022291-85-6	9

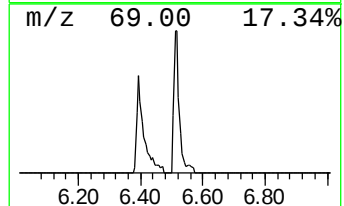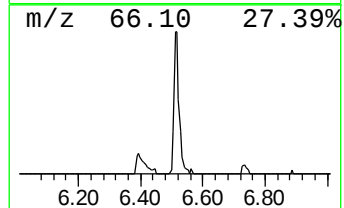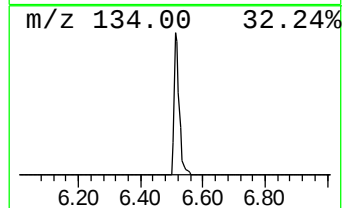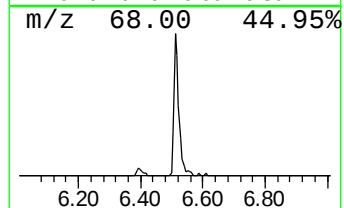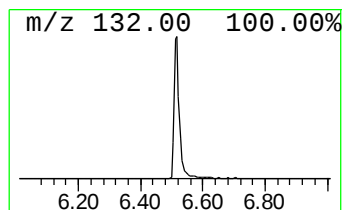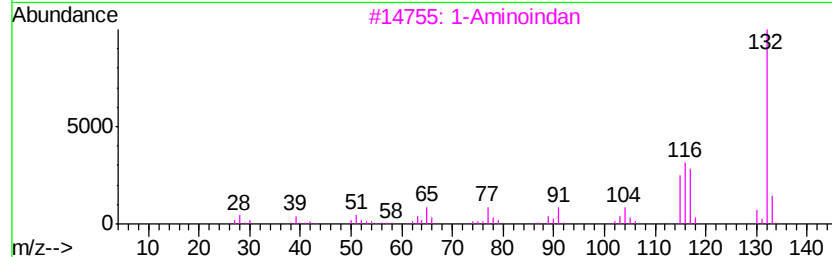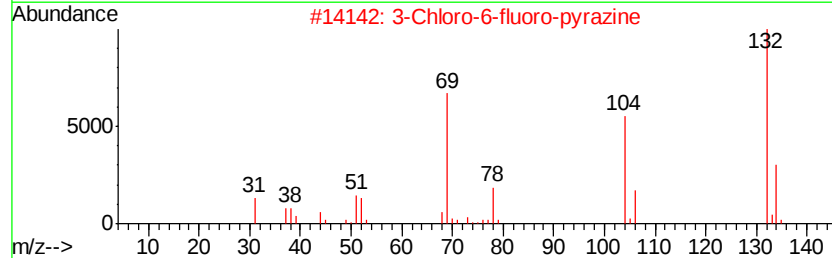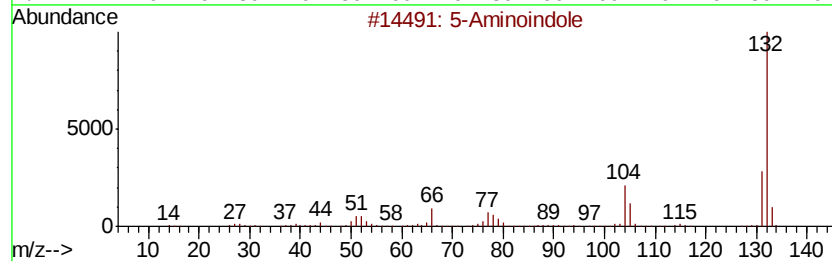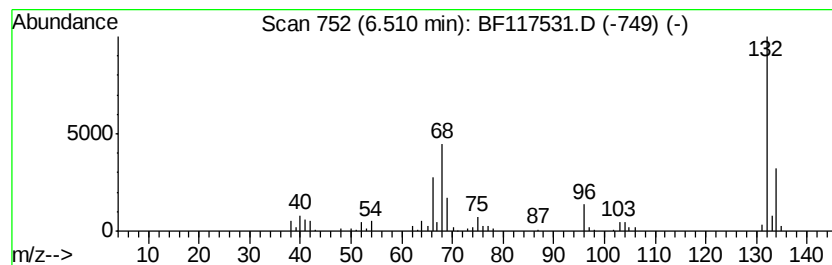

Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF102419\
Data File : BF117531.D
Acq On : 25 Oct 2019 00:39
Operator : JU
Sample : K5498-07 5X
Misc :
ALS Vial : 25 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
196-00-(0-1)

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF101819.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
unknown6.51	6.51	14.0	ng	189553	1	6.73	270504	20.0