


Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF102419\
 Data File : BF117507.D
 Acq On : 24 Oct 2019 13:50
 Operator : JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF101819.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Oct 18 18:53:31 2019

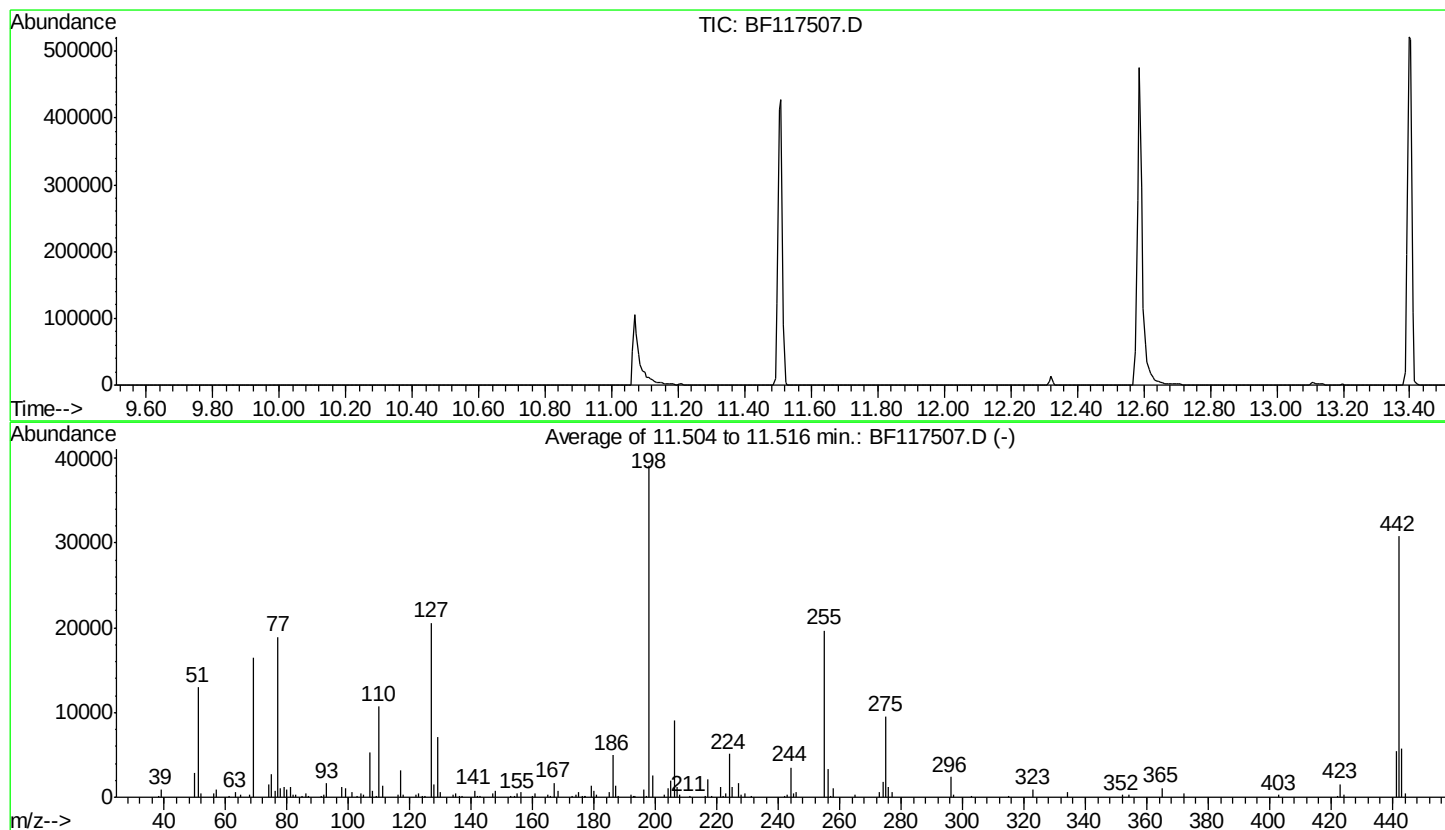

AutoFind: Scans 1601, 1602, 1603; Background Corrected with Scan 1596

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	33.1	12959	PASS
68	69	0.00	2	1.6	269	PASS
69	198	0.00	100	42.1	16462	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	52.6	20594	PASS
197	198	0.00	2	0.4	168	PASS
198	198	100	100	100.0	39144	PASS
199	198	5	9	6.6	2603	PASS
275	198	10	60	24.3	9494	PASS
365	198	1	100	2.8	1099	PASS
441	198	0.01	100	13.8	5413	PASS
442	198	50	100	78.6	30778	PASS
443	442	15	24	18.4	5677	PASS