
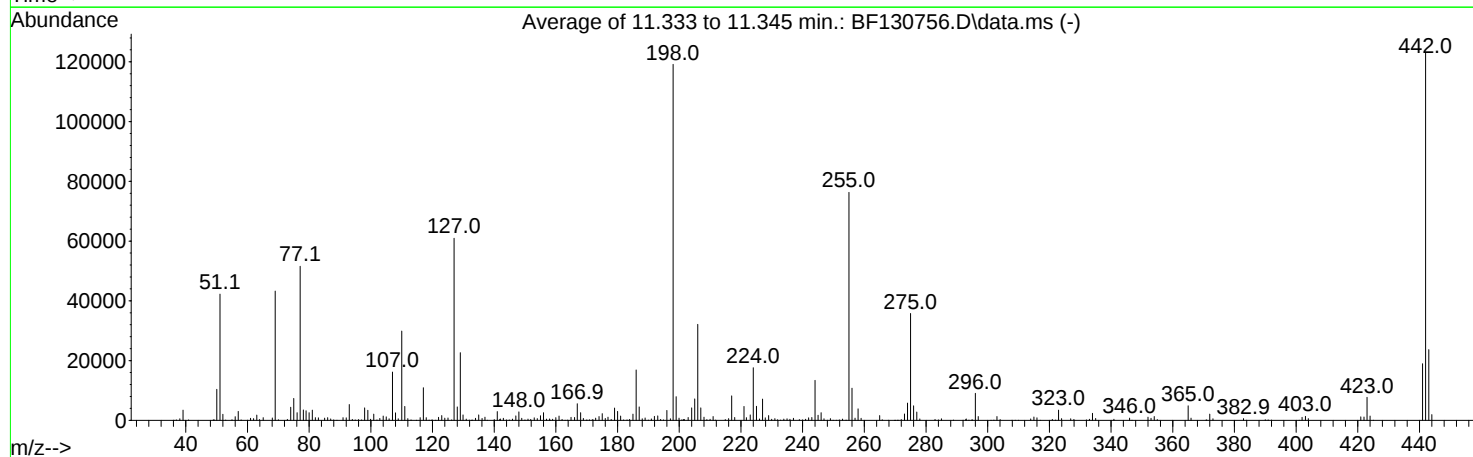


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF102422\
 Data File : BF130756.D
 Acq On : 24 Oct 2022 11:26
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF102022.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Oct 21 06:12:36 2022

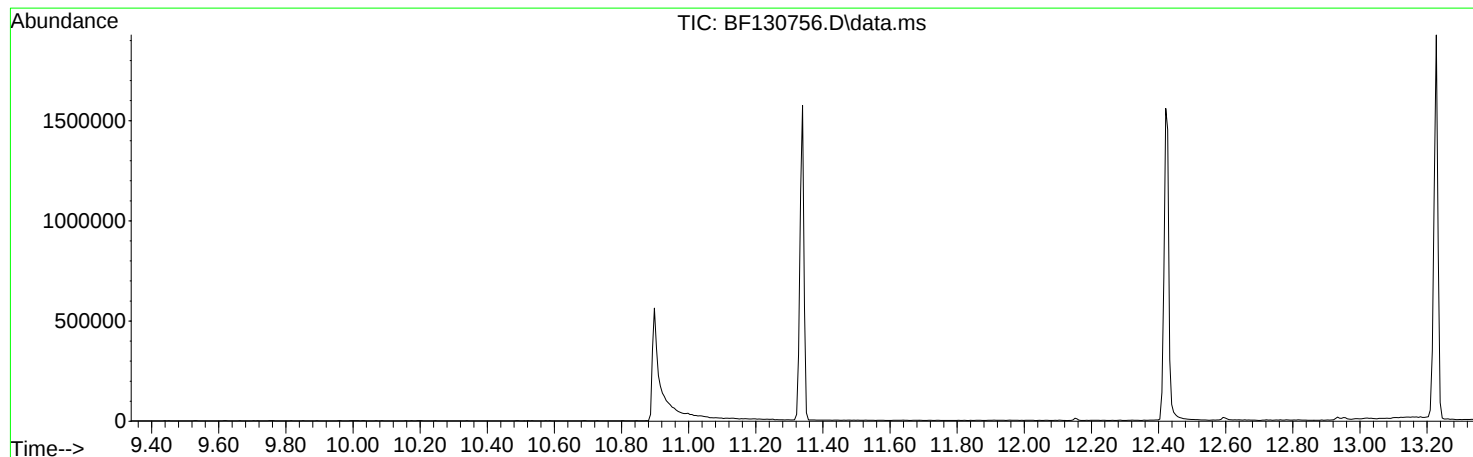




AutoFind: Scans 1606, 1607, 1608; Background Corrected with Scan 1601

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	35.5	42252	PASS
68	69	0.00	2	1.9	830	PASS
69	198	0.00	100	36.3	43254	PASS
70	69	0.00	2	0.5	200	PASS
127	198	10	80	51.1	60925	PASS
197	198	0.00	2	0.5	559	PASS
198	198	100	100	100.0	119120	PASS
199	198	5	9	6.6	7911	PASS
275	198	10	60	30.0	35789	PASS
365	198	1	100	4.1	4862	PASS
441	198	0.01	100	15.9	18981	PASS
442	442	50	100	100.0	123109	PASS
443	442	15	24	19.2	23689	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF102422\
Data File : BF130756.D
Acq On : 24 Oct 2022 11:26
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Oct 25 00:09:40 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF102022.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Oct 21 06:12:36 2022
Response via : Initial Calibration

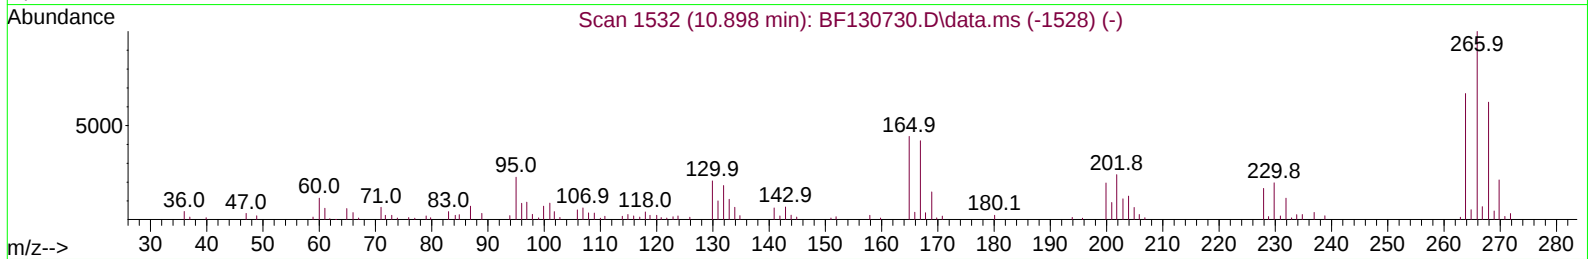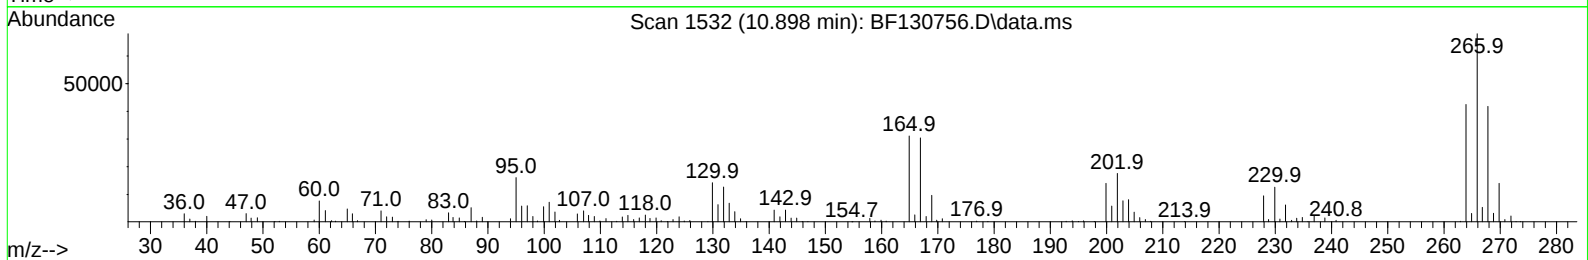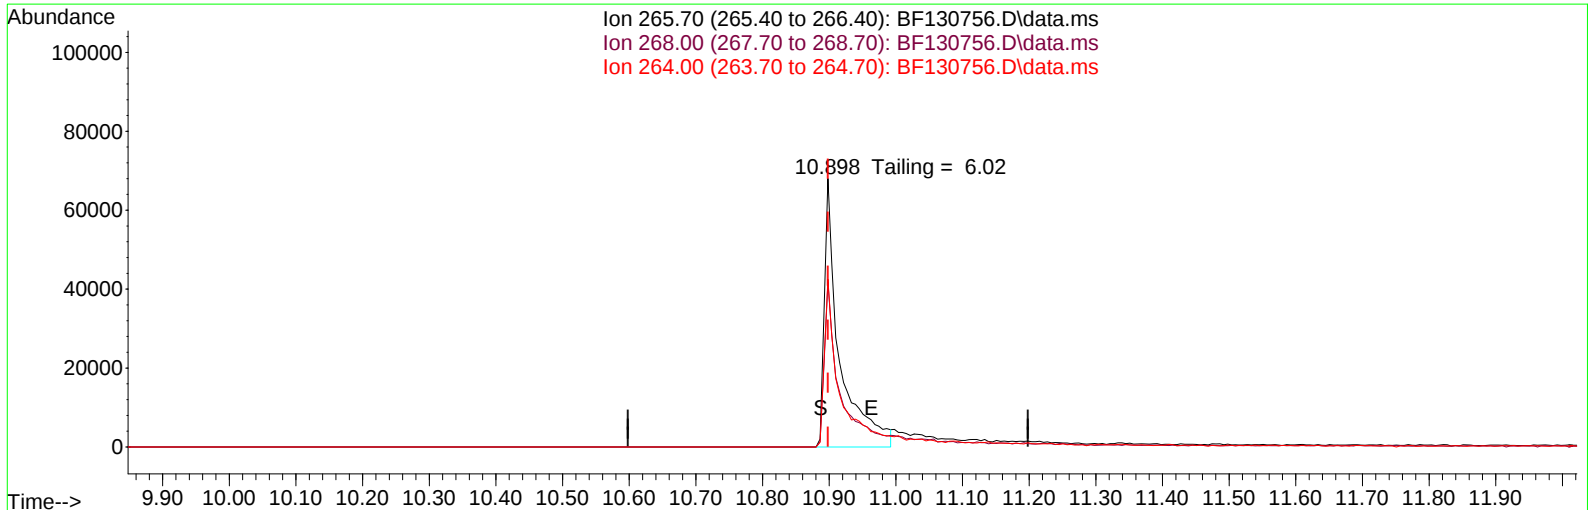

TIC: BF130756.D\data.ms

(70) Pentachlorophenol (C)




10.898min (+ 0.000) 11621.23 ng

response 115090

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.40	61.43
264.00	67.00	62.45
0.00	0.00	0.00

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Oct 25 00:09:40 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF102022.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Oct 21 06:12:36 2022
Response via : Initial Calibration

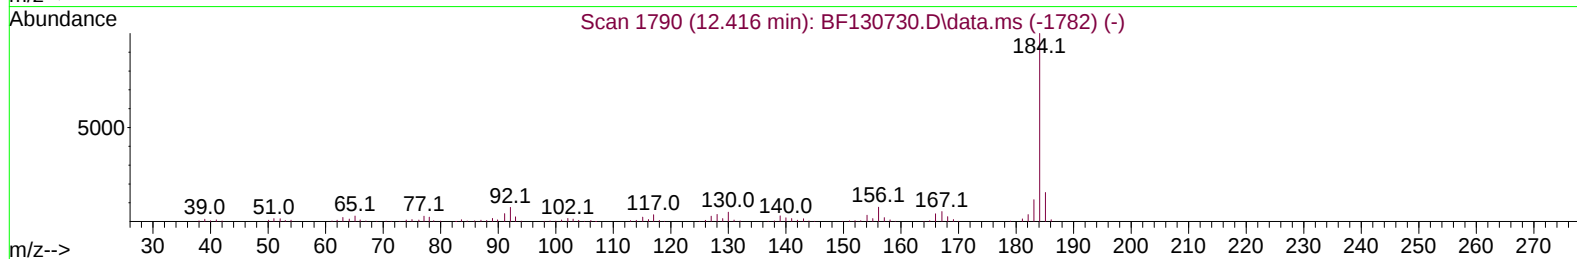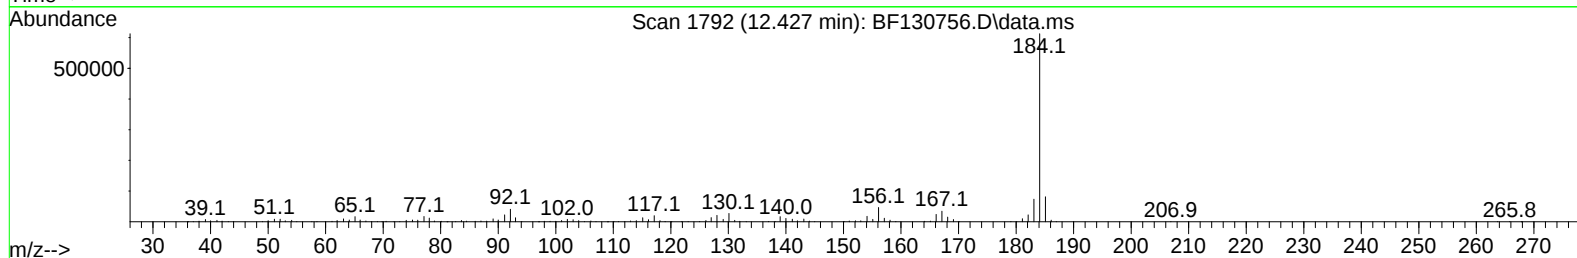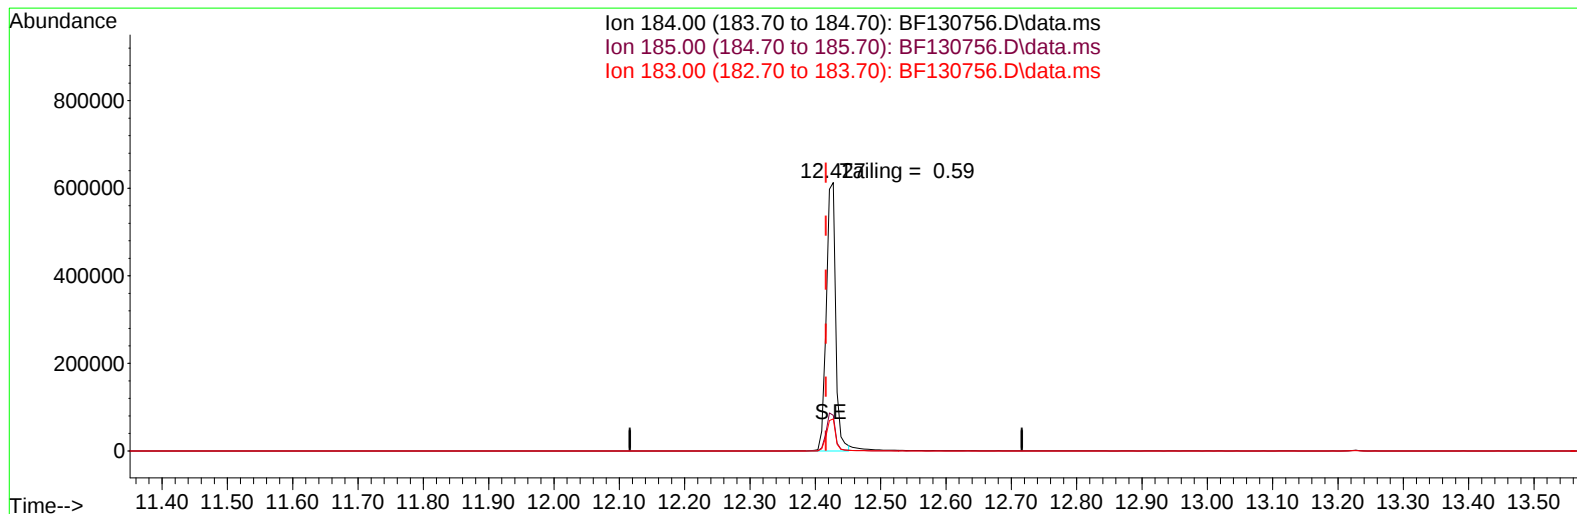

TIC: BF130756.D\data.ms

(77) Benzidine

12.427min (+ 0.011) 0.00 ng

response **626755**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	13.28
183.00	11.60	11.96
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
10/24/2022	BNA_F	<u>BF130756.D</u>
Compound Name	Response	Retention Time
DDT	295397	13.227
DDD	5240	12.933
DDE	3142	12.592
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
8382	303779	2.76

Instrument :
BNA_F
ClientSampleId :
DFTPP