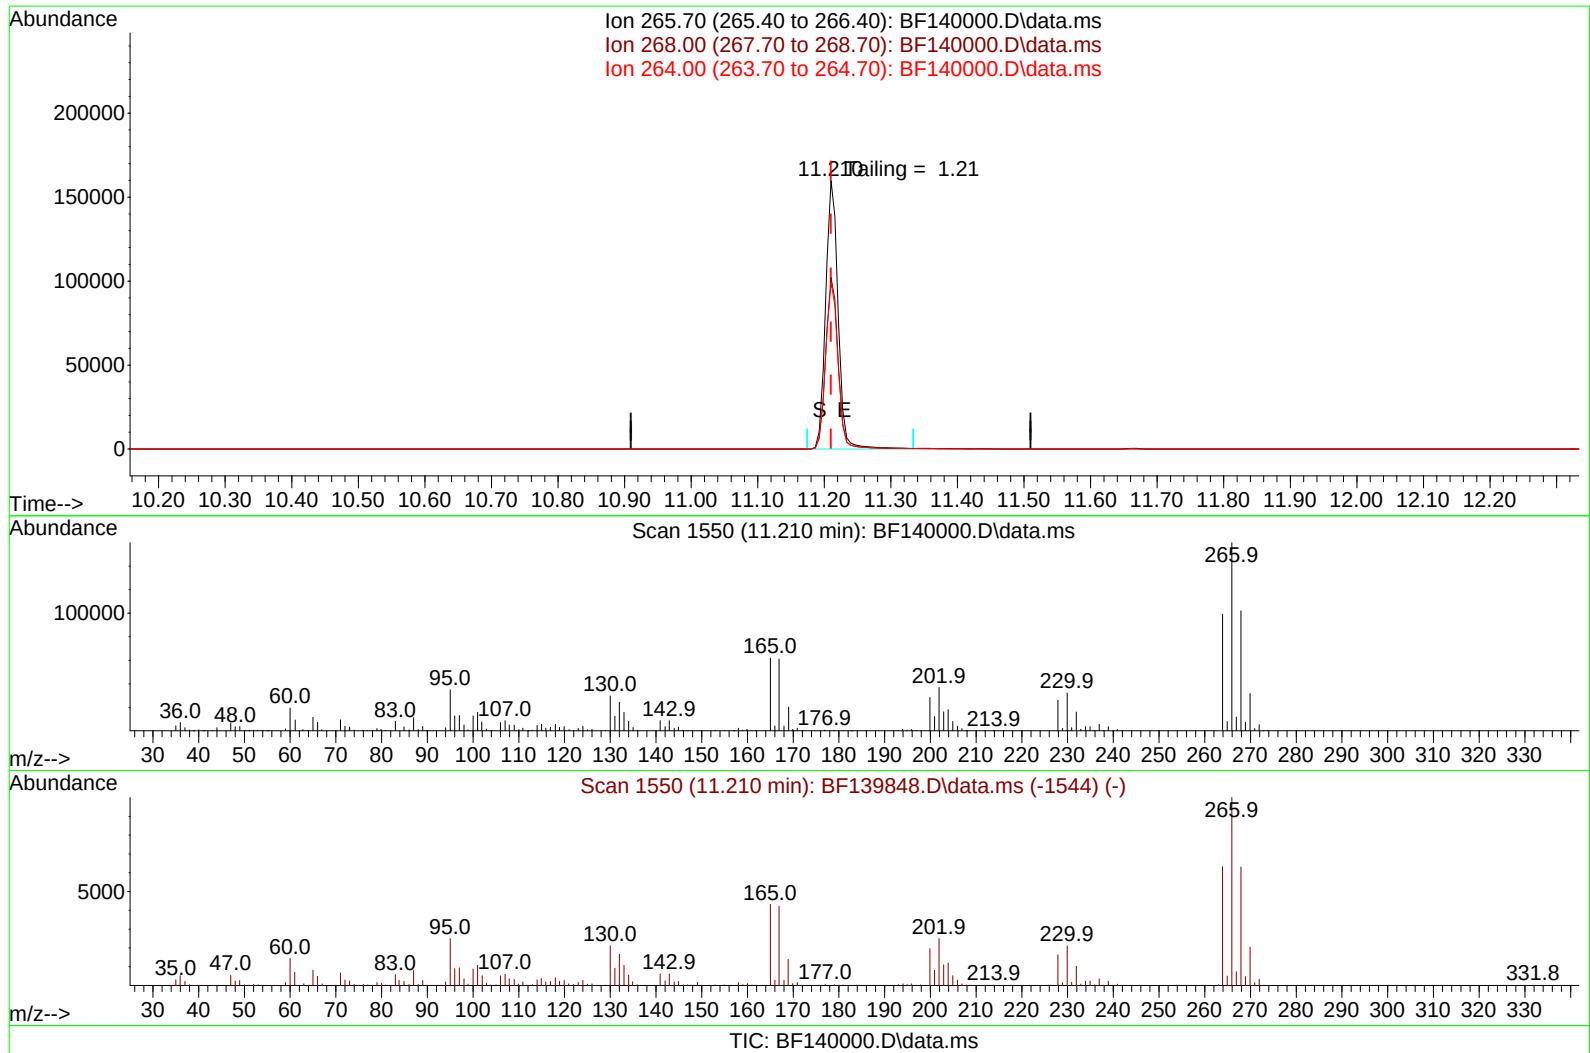


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF102424\
Data File : BF140000.D
Acq On : 24 Oct 2024 14:47
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1




Quant Time: Oct 24 15:14:24 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF101824.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Oct 18 15:07:50 2024
Response via : Initial Calibration

**(70) Pentachlorophenol (C)****11.210min (+ 0.000) 39709.65 ng****response 208862**

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.00	63.86
264.00	63.20	62.10
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF102424\
Data File : BF140000.D
Acq On : 24 Oct 2024 14:47
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 24 15:14:24 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF101824.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Oct 18 15:07:50 2024
Response via : Initial Calibration

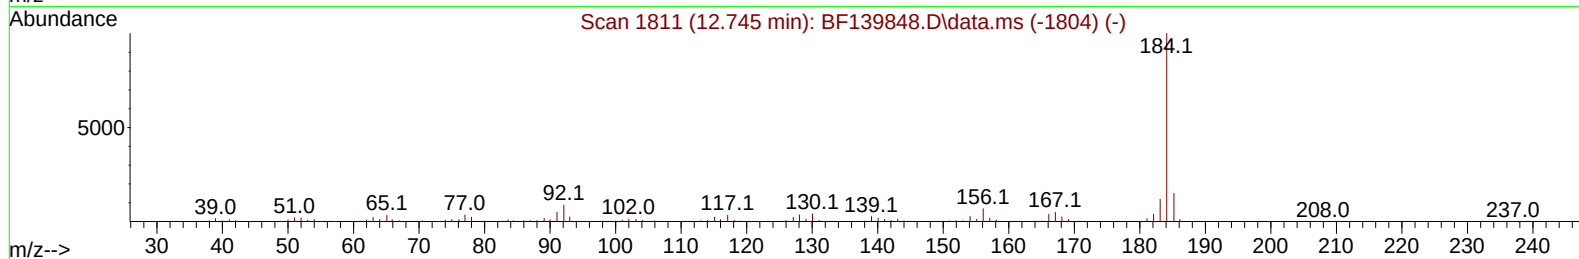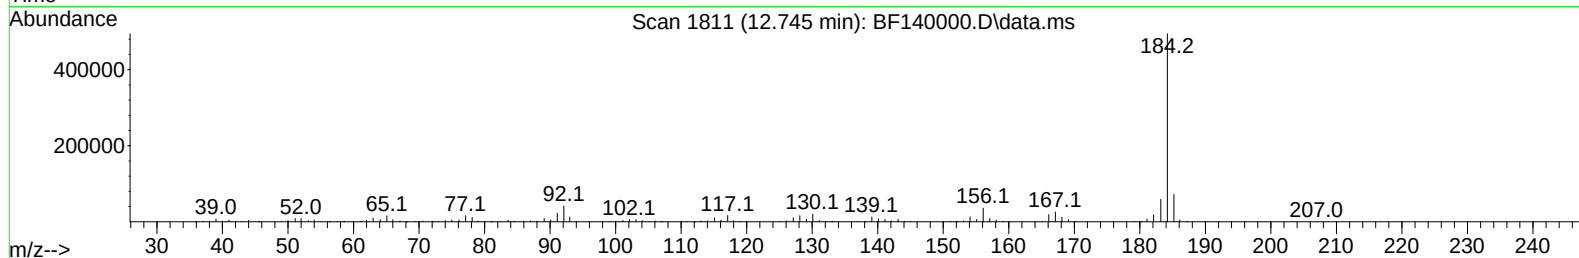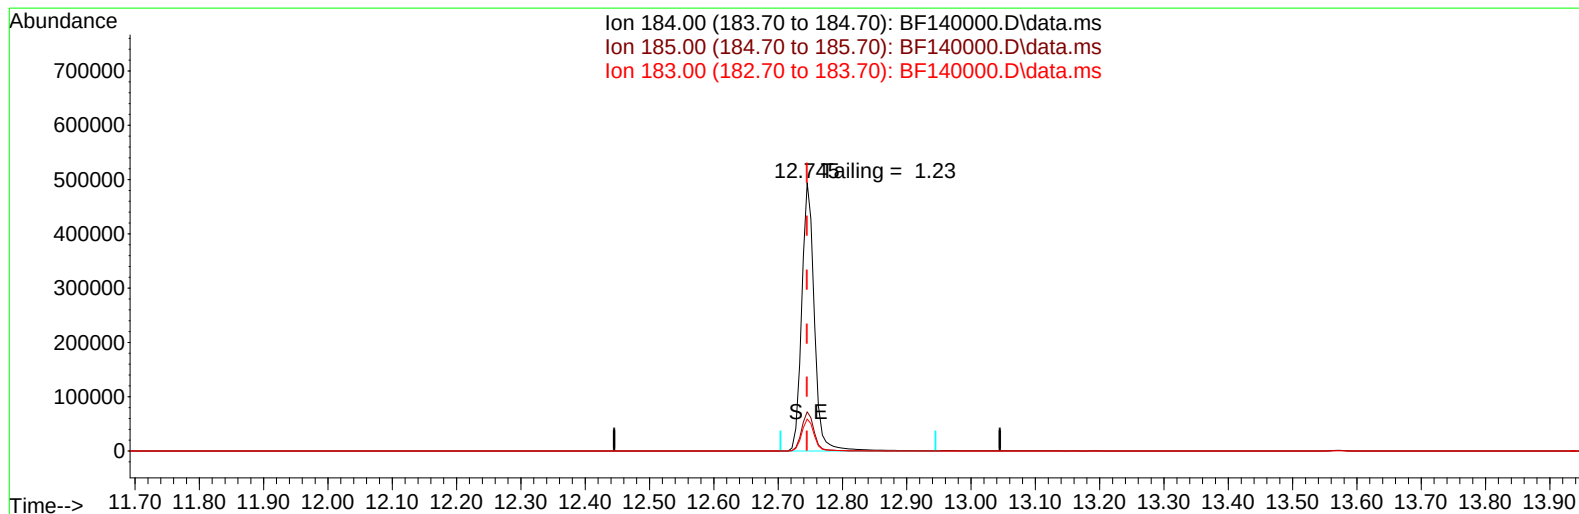

TIC: BF140000.D\data.ms

(77) Benzidine

12.745min (+ 0.000) 156375.06 ng

response 678833

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.00	14.62
183.00	11.80	11.94
0.00	0.00	0.00