

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF102424\
 Data File : BF140013.D
 Acq On : 24 Oct 2024 21:04
 Operator : RC/JU
 Sample : P4467-01
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 TP-1

Quant Time: Oct 25 01:09:36 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF101824.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Oct 18 15:07:50 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	6.887	152	79395	20.000	ng	0.00
21) Naphthalene-d8	8.169	136	294278	20.000	ng	0.00
39) Acenaphthene-d10	9.922	164	157029	20.000	ng	0.00
64) Phenanthrene-d10	11.410	188	245482	20.000	ng	0.00
76) Chrysene-d12	14.045	240	142405	20.000	ng	0.00
86) Perylene-d12	15.527	264	182835	20.000	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.504	112	521666	102.861	ng	0.00
7) Phenol-d6	6.504	99	642008	97.740	ng	0.00
23) Nitrobenzene-d5	7.445	82	434467	81.826	ng	0.00
42) 2,4,6-Tribromophenol	10.710	330	160215	109.079	ng	0.00
45) 2-Fluorobiphenyl	9.245	172	741220	78.012	ng	0.00
79) Terphenyl-d14	12.992	244	548459	62.758	ng	0.00


Target Compounds	Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF102424\
Data File : BF140013.D
Acq On : 24 Oct 2024 21:04
Operator : RC/JU
Sample : P4467-01
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
TP-1

Quant Time: Oct 25 01:09:36 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF101824.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Oct 18 15:07:50 2024
Response via : Initial Calibration



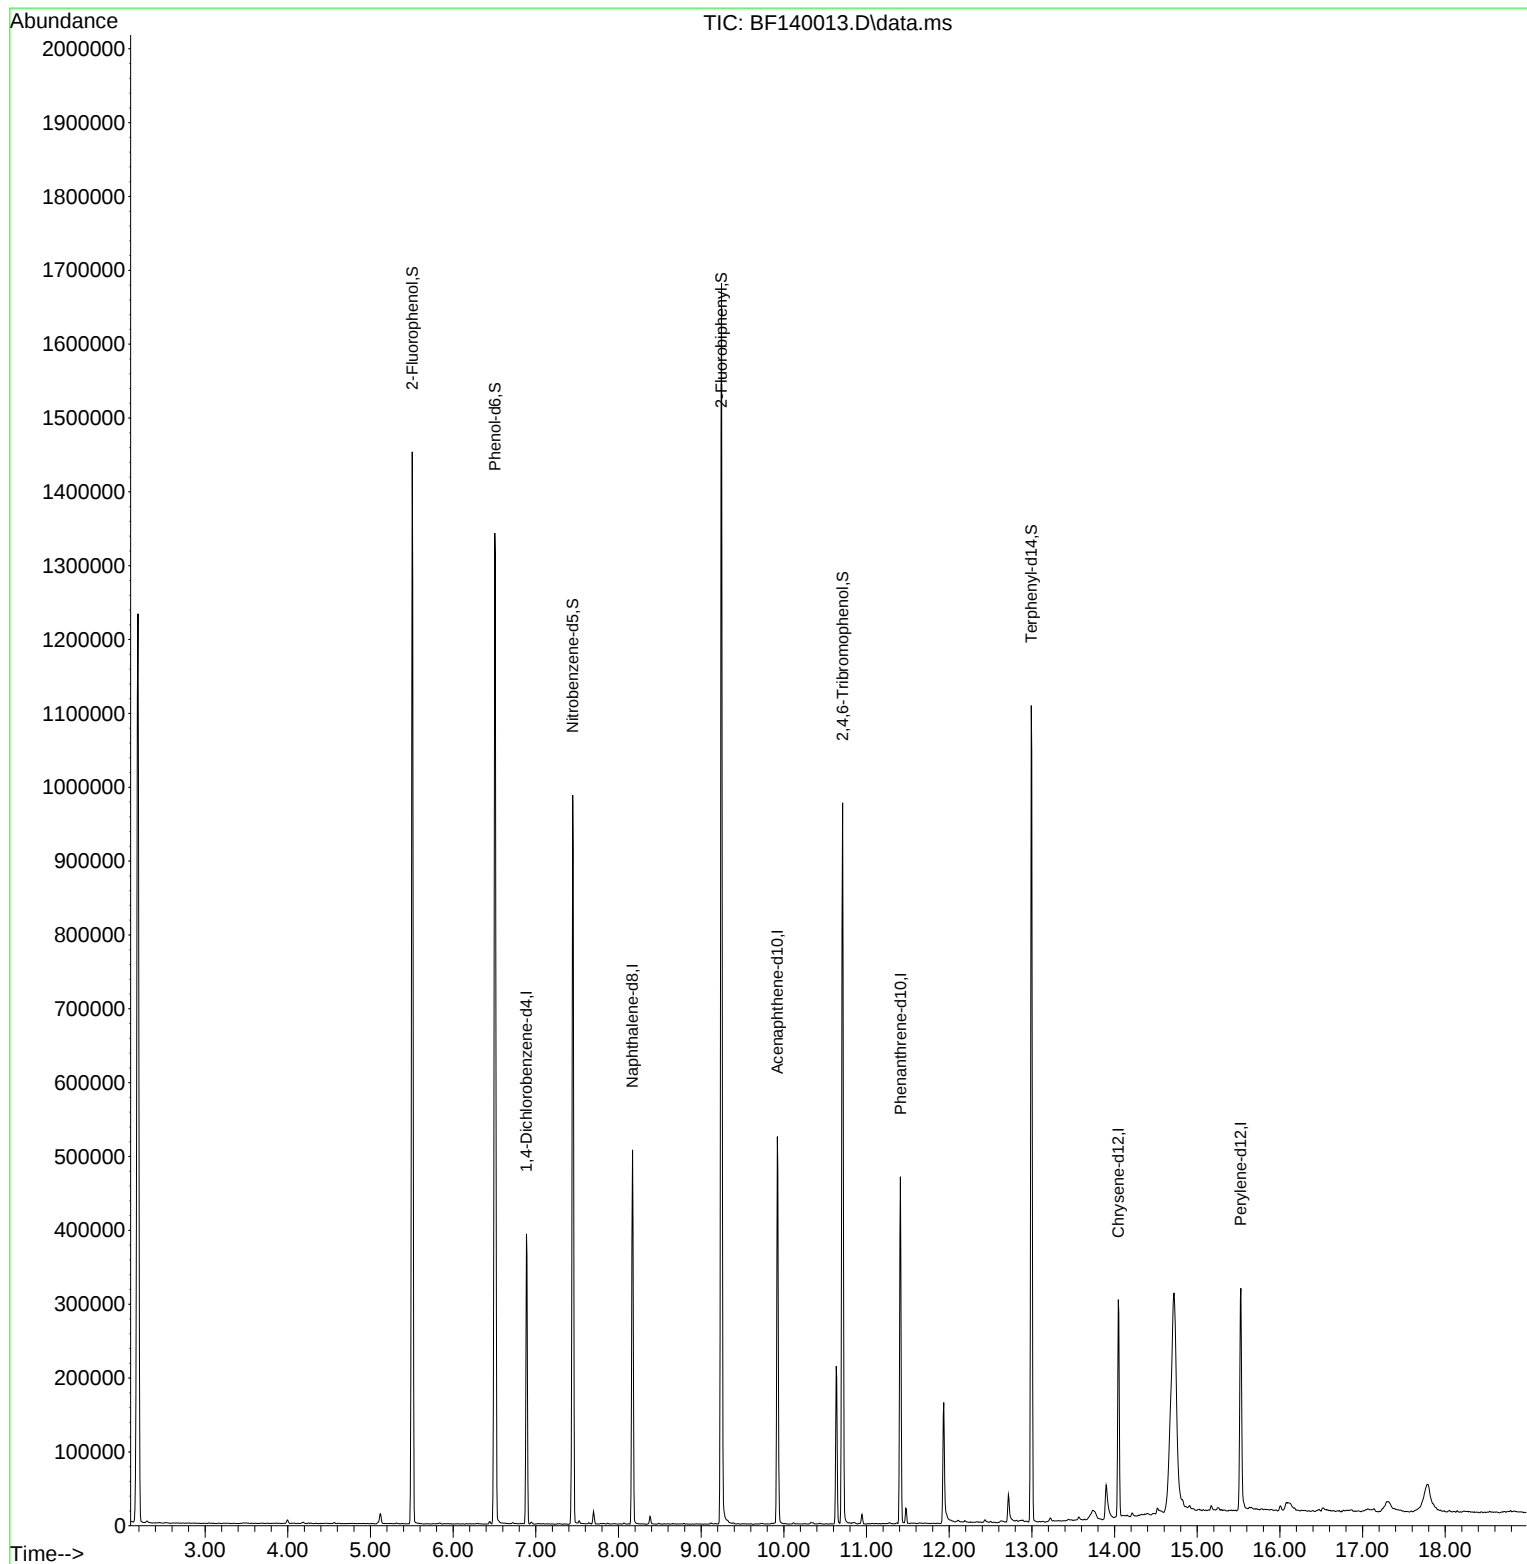




#1
1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 6.887 min Scan# 816
Delta R.T. -0.005 min
Lab File: BF140013.D
Acq: 24 Oct 2024 21:04




Instrument :
BNA_F
ClientSampleId :
TP-1

Tgt Ion:152 Resp: 79395
Ion Ratio Lower Upper
152 100
150 155.5 130.2 195.2
115 63.4 51.4 77.2

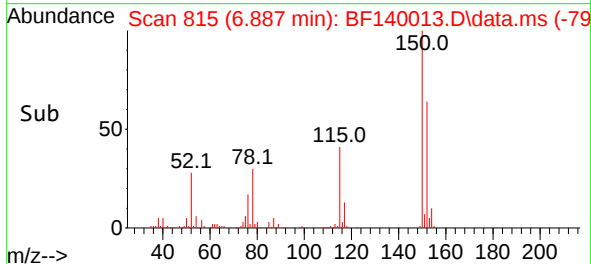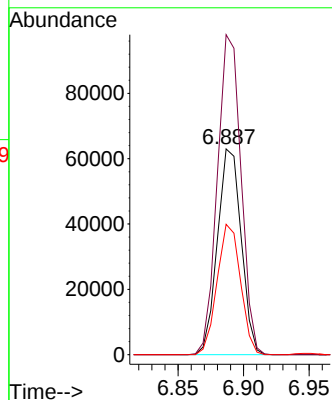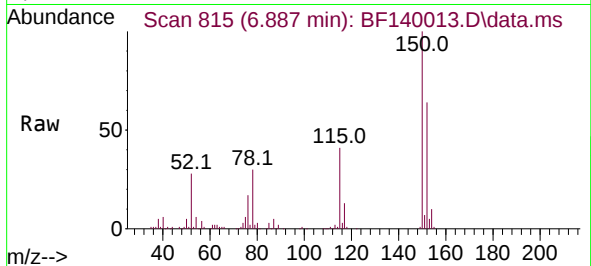

#5
2-Fluorophenol
Concen: 102.861 ng
RT: 5.504 min Scan# 580
Delta R.T. 0.006 min
Lab File: BF140013.D
Acq: 24 Oct 2024 21:04

Tgt Ion:112 Resp: 521666
Ion Ratio Lower Upper
112 100
64 64.5 53.0 79.6
63 35.2 27.0 40.4

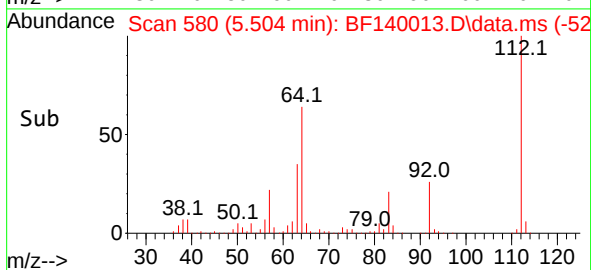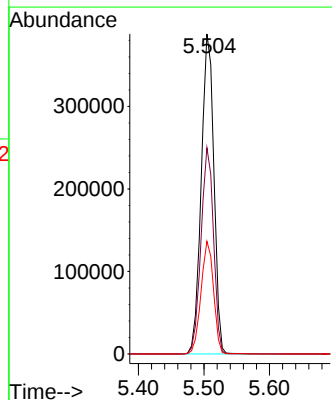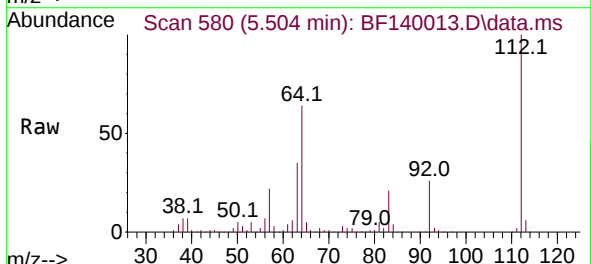



#7

Phenol-d6

Concen: 97.740 ng

RT: 6.504 min Scan# 71

Delta R.T. -0.006 min

Lab File: BF140013.D

Acq: 24 Oct 2024 21:04

Instrument :

BNA_F

ClientSampleId :

TP-1





Tgt Ion: 99 Resp: 642008

Ion Ratio Lower Upper

99 100

42 21.2 16.7 25.1

71 38.3 27.7 41.5

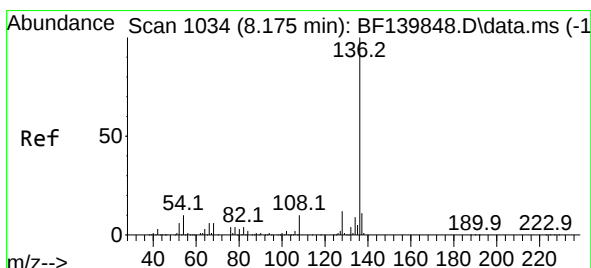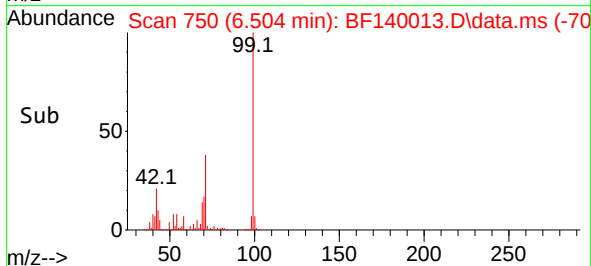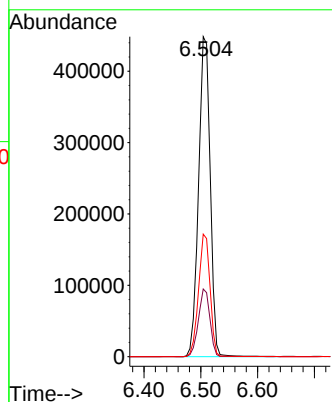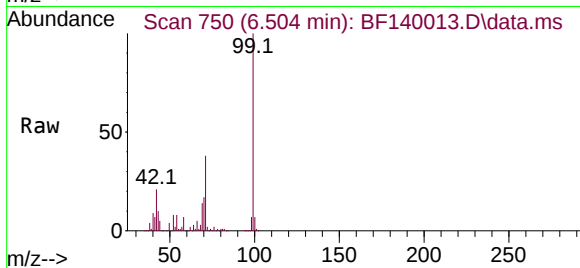

#21

Naphthalene-d8

Concen: 20.000 ng

RT: 8.169 min Scan# 1033

Delta R.T. -0.006 min

Lab File: BF140013.D

Acq: 24 Oct 2024 21:04

Tgt Ion: 136 Resp: 294278




Ion Ratio Lower Upper


136 100

137 10.9 8.6 12.8

54 9.3 8.4 12.6

68 5.7 5.1 7.7


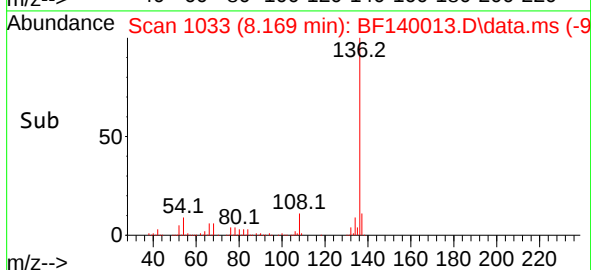
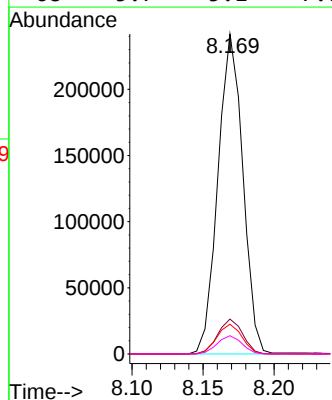
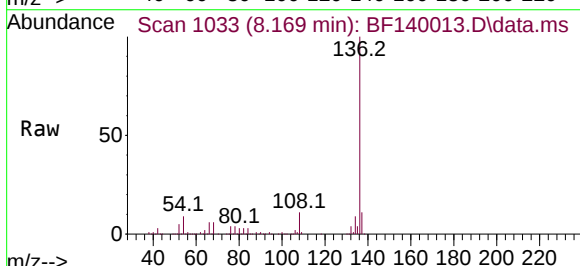


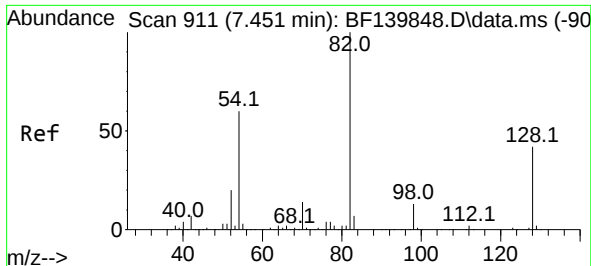

#23
Nitrobenzene-d5
Concen: 81.826 ng
RT: 7.445 min Scan# 911
Delta R.T. -0.006 min
Lab File: BF140013.D
Acq: 24 Oct 2024 21:04




Instrument :
BNA_F
ClientSampleId :
TP-1

Tgt Ion: 82 Resp: 434467
Ion Ratio Lower Upper
82 100
128 41.2 33.4 50.0
54 57.7 47.8 71.8

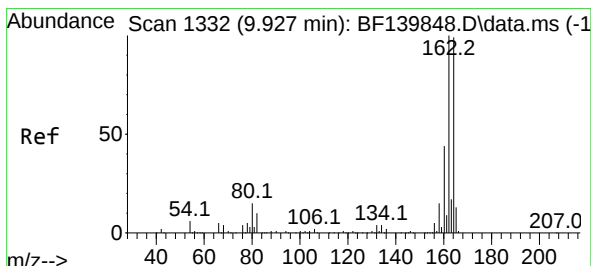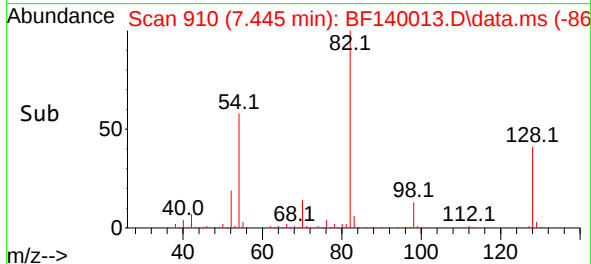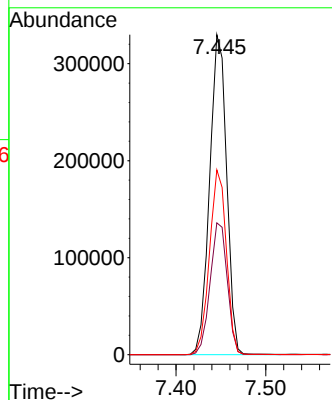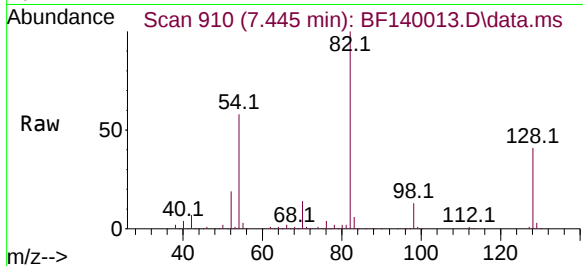

#39
Acenaphthene-d10
Concen: 20.000 ng
RT: 9.922 min Scan# 1331
Delta R.T. -0.005 min
Lab File: BF140013.D
Acq: 24 Oct 2024 21:04

Tgt Ion: 164 Resp: 157029
Ion Ratio Lower Upper
164 100
162 101.1 81.0 121.4
160 45.2 35.4 53.0


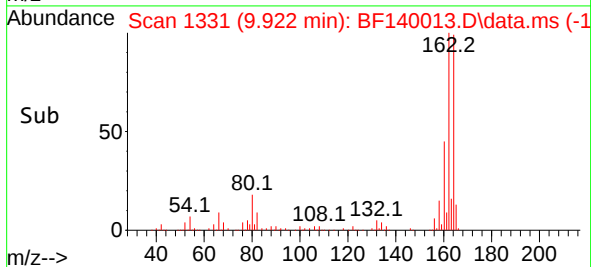
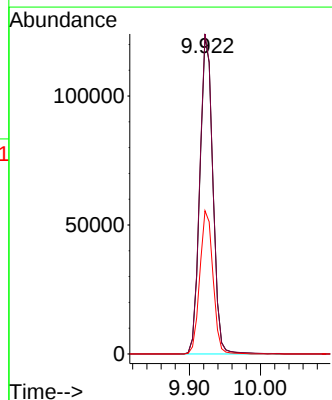
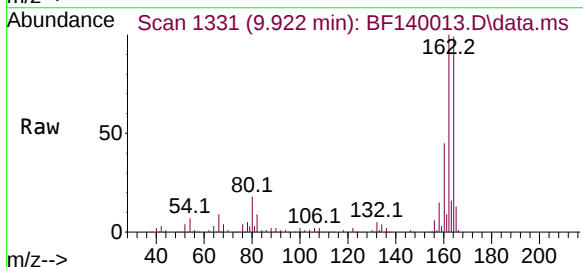




#42
2,4,6-Tribromophenol
Concen: 109.079 ng
RT: 10.710 min Scan# 1465
Delta R.T. -0.006 min
Lab File: BF140013.D
Acq: 24 Oct 2024 21:04




Instrument :
BNA_F
ClientSampleId :
TP-1


Tgt Ion:330 Resp: 160215
Ion Ratio Lower Upper
330 100
332 97.0 78.1 117.1
141 31.0 26.6 39.8

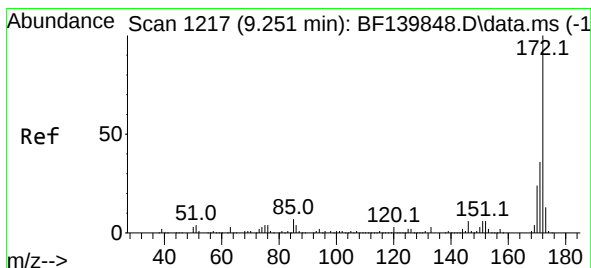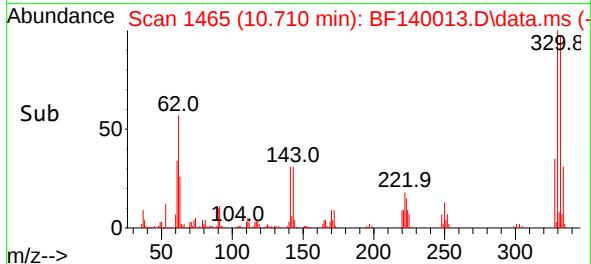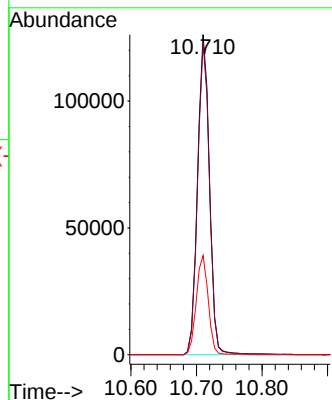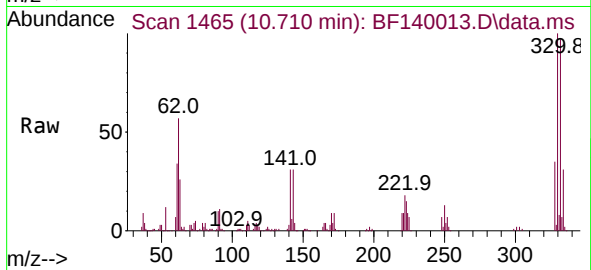

#45
2-Fluorobiphenyl
Concen: 78.012 ng
RT: 9.245 min Scan# 1216
Delta R.T. -0.006 min
Lab File: BF140013.D
Acq: 24 Oct 2024 21:04

Tgt Ion:172 Resp: 741220
Ion Ratio Lower Upper
172 100
171 35.2 28.6 43.0
170 23.5 19.1 28.7

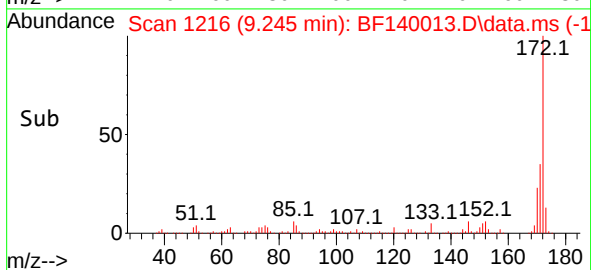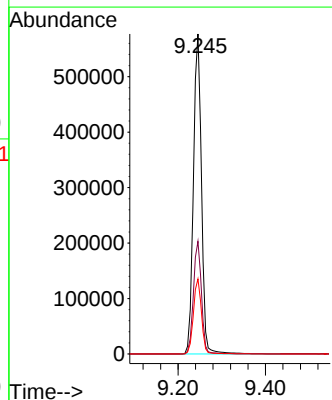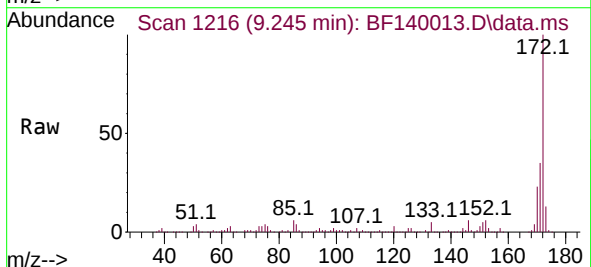

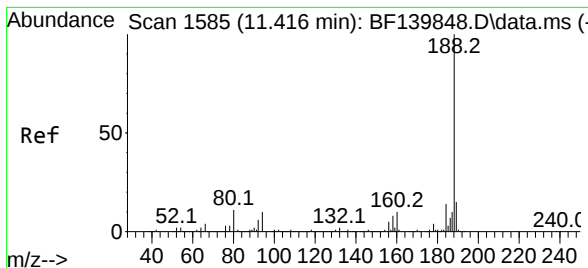

#64

Phenanthrene-d10

Concen: 20.000 ng

RT: 11.410 min Scan# 1

Delta R.T. -0.006 min

Lab File: BF140013.D

Acq: 24 Oct 2024 21:04

Instrument :

BNA_F

ClientSampleId :

TP-1





Tgt Ion:188 Resp: 245482

Ion Ratio Lower Upper

188 100

94 8.9 7.9 11.9

80 9.7 9.0 13.4

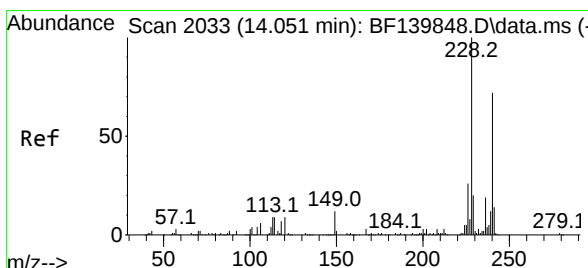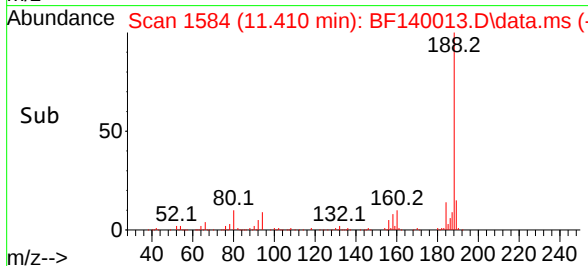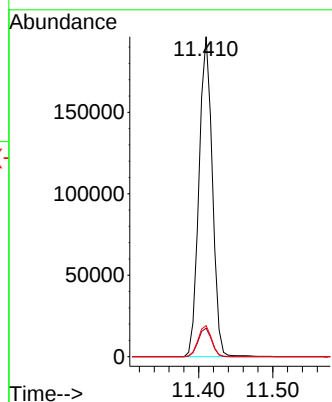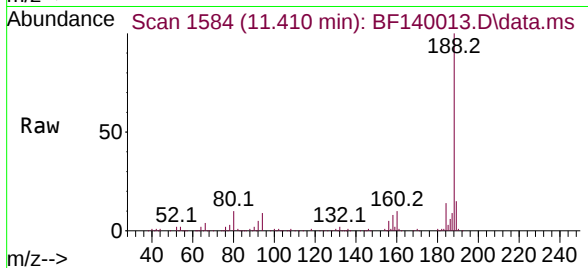

#76

Chrysene-d12

Concen: 20.000 ng

RT: 14.045 min Scan# 2032

Delta R.T. -0.006 min

Lab File: BF140013.D

Acq: 24 Oct 2024 21:04




Tgt Ion:240 Resp: 142405


Ion Ratio Lower Upper

240 100

120 10.1 9.4 14.2

236 25.7 20.9 31.3


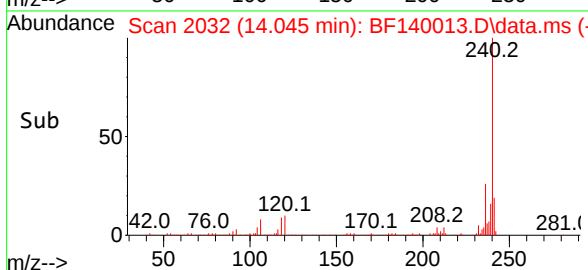
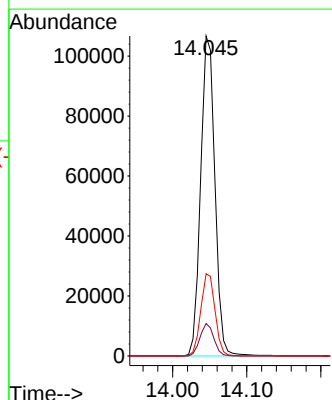
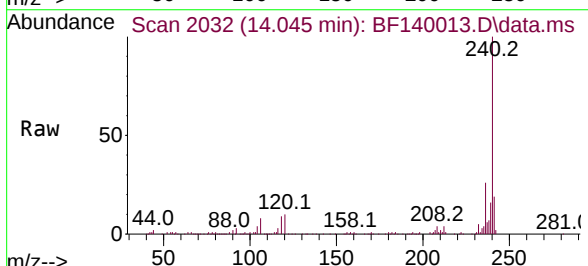


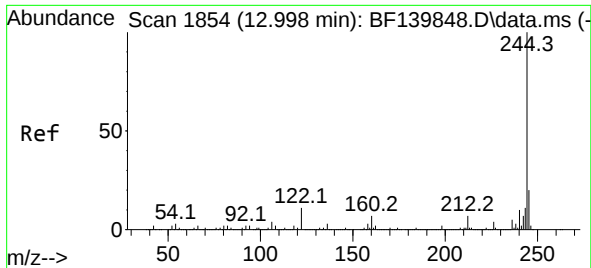

#79
 Terphenyl-d14
 Concen: 62.758 ng
 RT: 12.992 min Scan# 1853
 Delta R.T. -0.006 min
 Lab File: BF140013.D
 Acq: 24 Oct 2024 21:04

Instrument :
 BNA_F
 ClientSampleId :
 TP-1

Tgt Ion:244 Resp: 548459
 Ion Ratio Lower Upper
 244 100
 212 7.0 5.7 8.5
 122 10.2 8.6 13.0

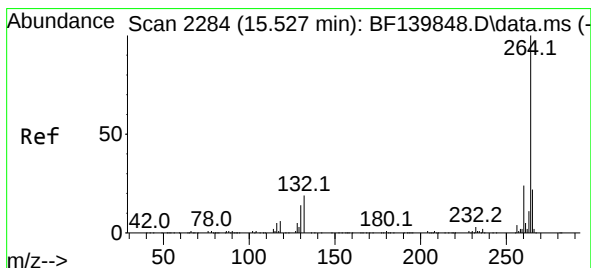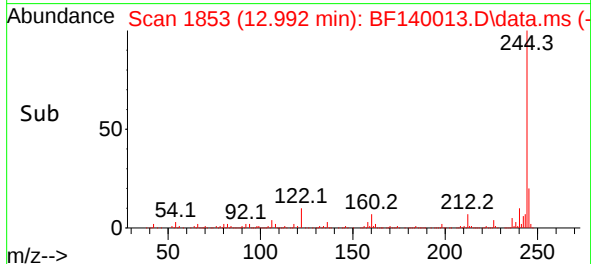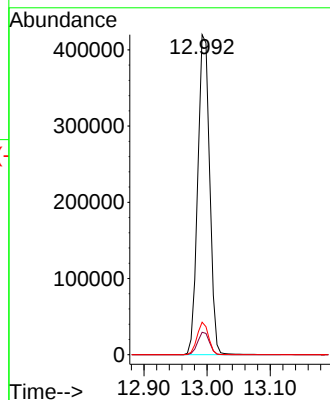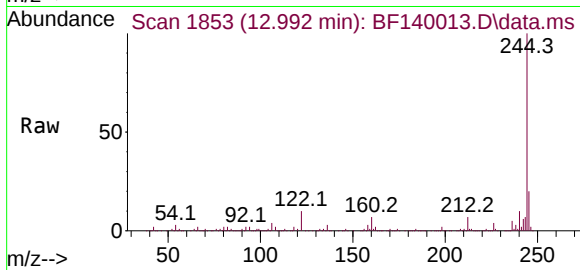

#86
 Perylene-d12
 Concen: 20.000 ng
 RT: 15.527 min Scan# 2284
 Delta R.T. 0.000 min
 Lab File: BF140013.D
 Acq: 24 Oct 2024 21:04

Tgt Ion:264 Resp: 182835
 Ion Ratio Lower Upper
 264 100
 260 23.3 19.4 29.2
 265 20.3 17.4 26.0

