
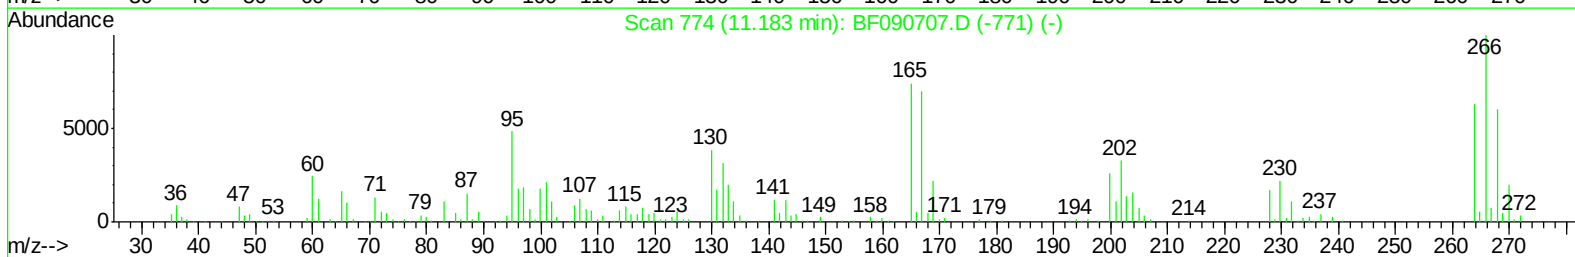
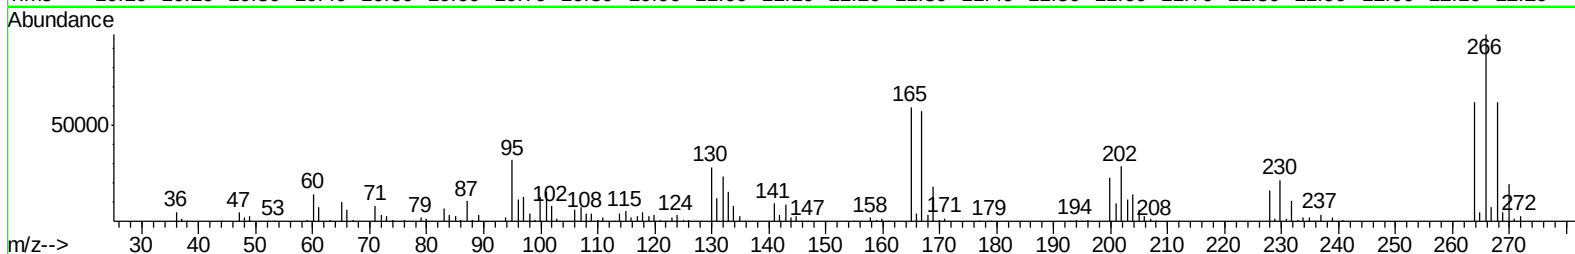


Data Path : Z:\HPCHEM1\BNA_F\DATA\BF102516\
Data File : BF090807.D
Acq On : 25 Oct 2016 15:15
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 25 18:43:03 2016
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF102116.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Oct 25 17:09:27 2016
Response via : Initial Calibration

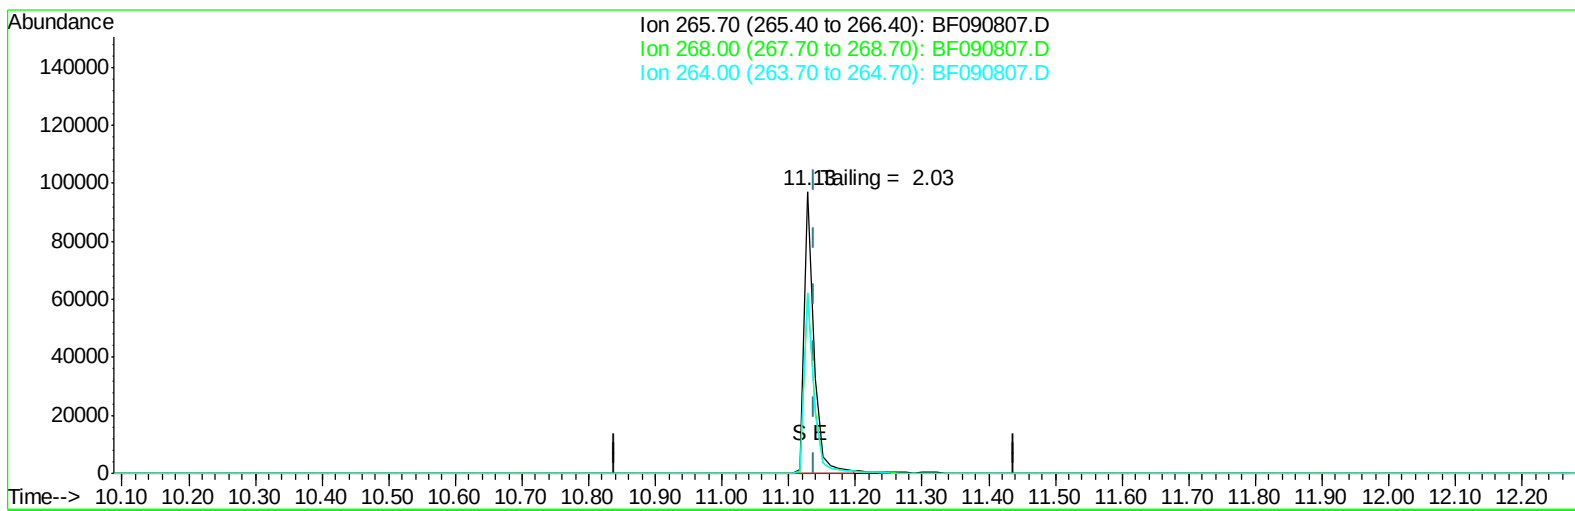

TIC: BF090807.D

(69) Pentachlorophenol (C)




11.128min (-0.011) 0.00ng

response 101081

Ion	Exp%	Act%
265.70	100	100
268.00	62.20	64.04
264.00	62.70	63.97
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF102516\
Data File : BF090807.D
Acq On : 25 Oct 2016 15:15
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 25 18:43:03 2016
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF102116.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Oct 25 17:09:27 2016
Response via : Initial Calibration

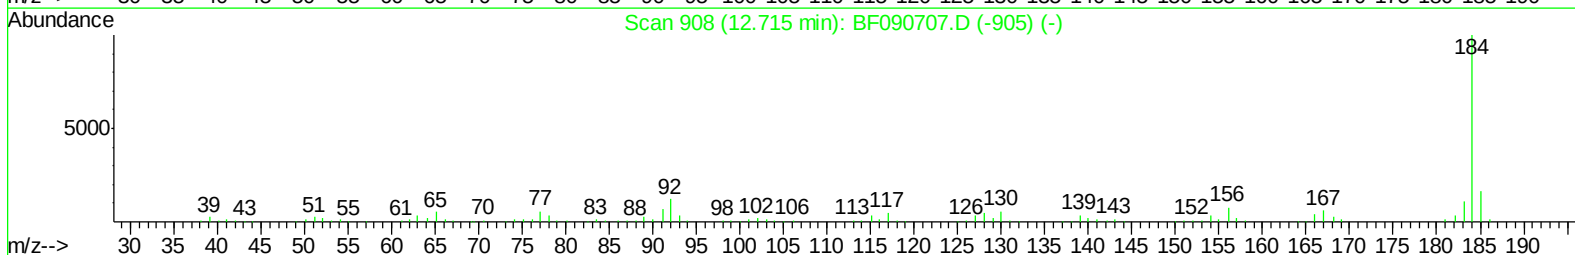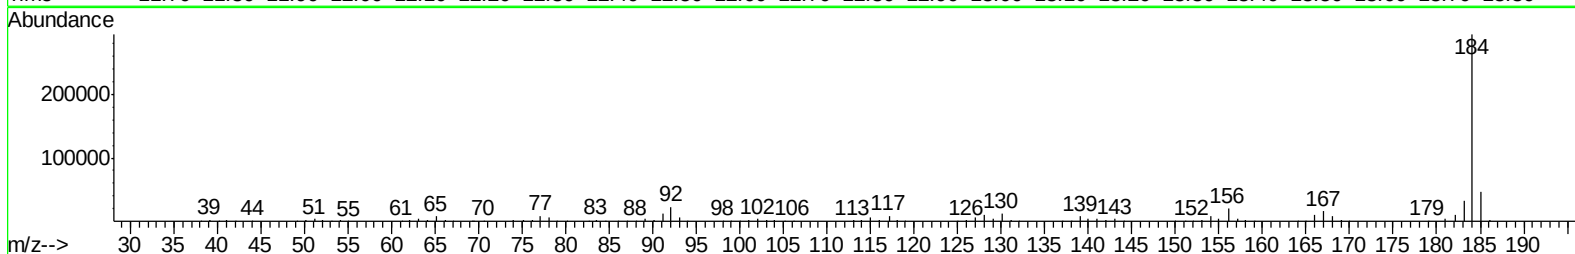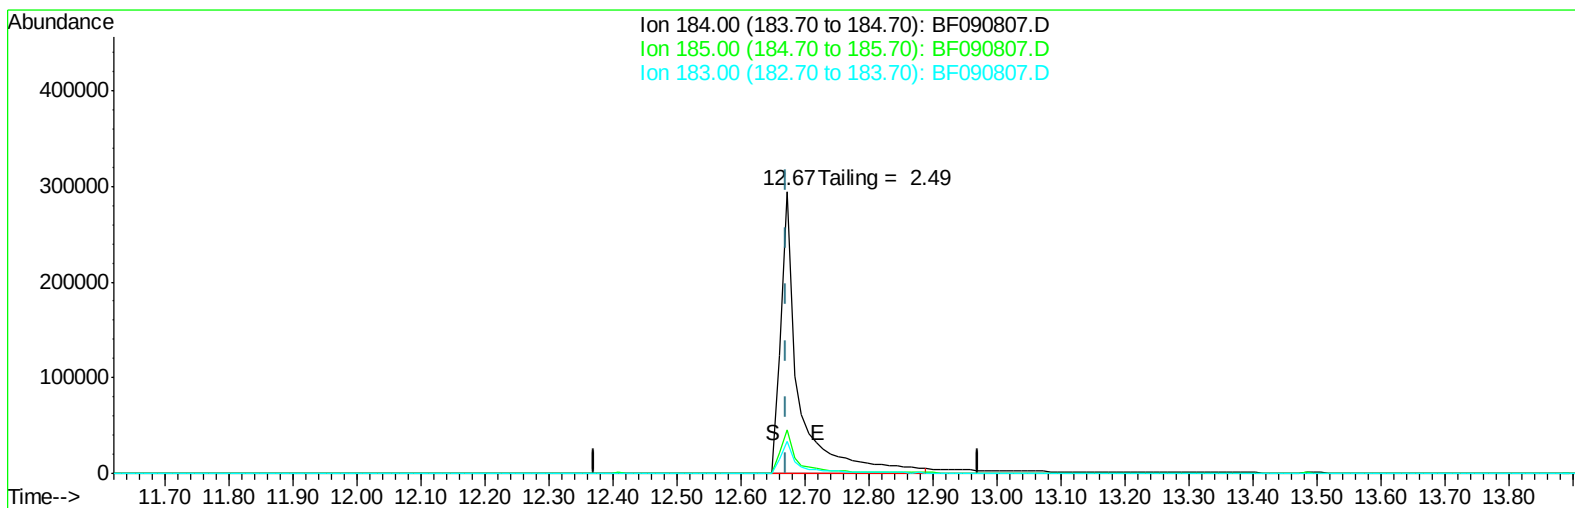

TIC: BF090807.D

(76) Benzidine

12.671min (+0.000) 0.00ng

response 573024

Ion	Exp%	Act%
184.00	100	100
185.00	14.70	15.64
183.00	9.50	11.29
0.00	0.00	0.00