


Data Path : Z:\HPCHEM1\BNA F\DATA\BF102516\
 Data File : BF090807.D
 Acq On : 25 Oct 2016 15:15
 Operator : UM/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF102116.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Oct 25 18:56:36 2016

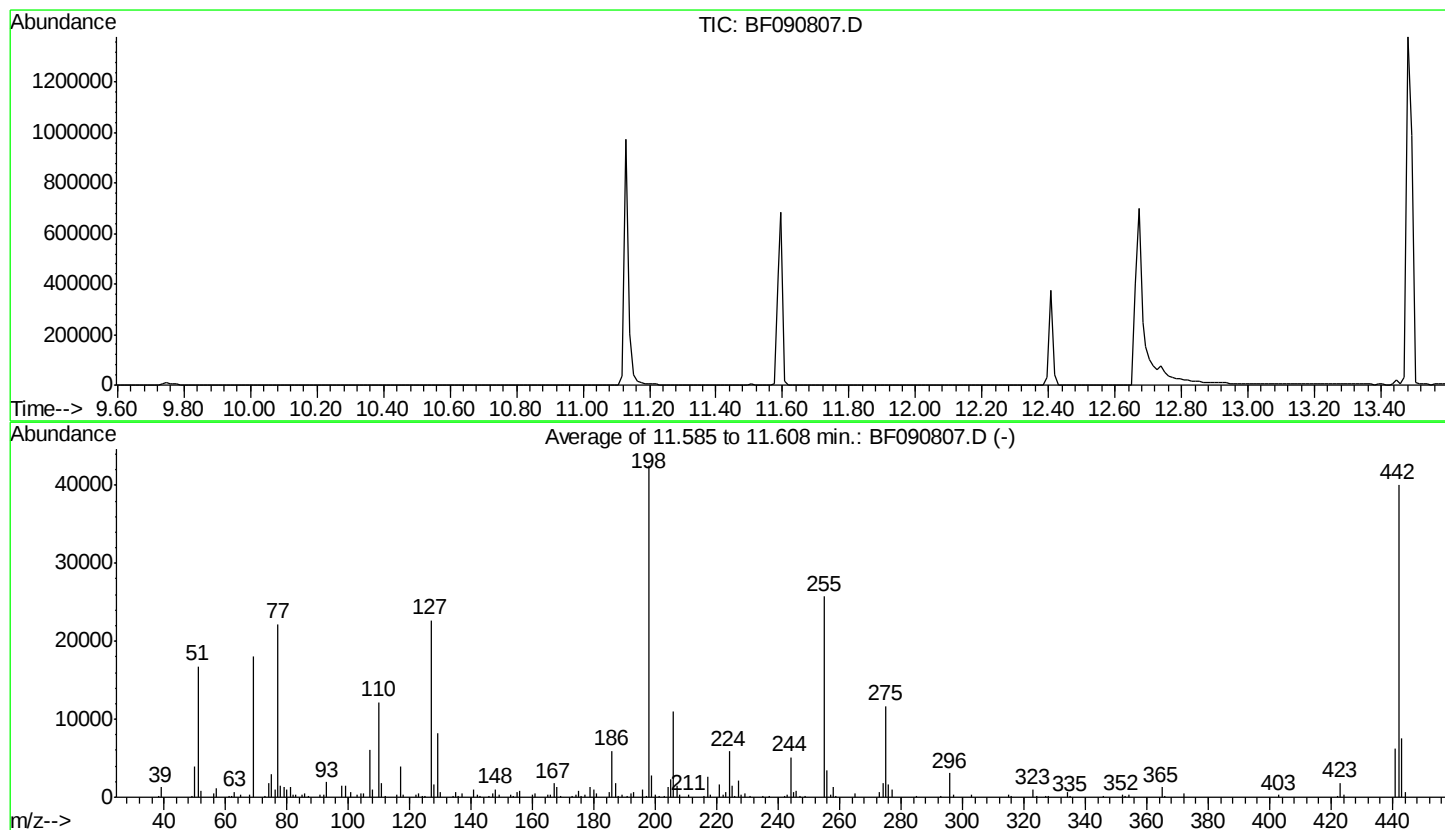

AutoFind: Scans 831, 832, 833; Background Corrected with Scan 827

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	39.4	16754	PASS
68	69	0.00	2	1.7	305	PASS
69	198	0.00	100	42.5	18082	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	53.4	22698	PASS
197	198	0.00	2	0.2	100	PASS
198	198	100	100	100.0	42528	PASS
199	198	5	9	6.8	2876	PASS
275	198	10	60	27.6	11724	PASS
365	198	1	100	3.0	1291	PASS
441	442	0.01	24	15.6	6261	PASS
442	198	50	100	94.4	40142	PASS
443	442	15	24	18.8	7557	PASS