
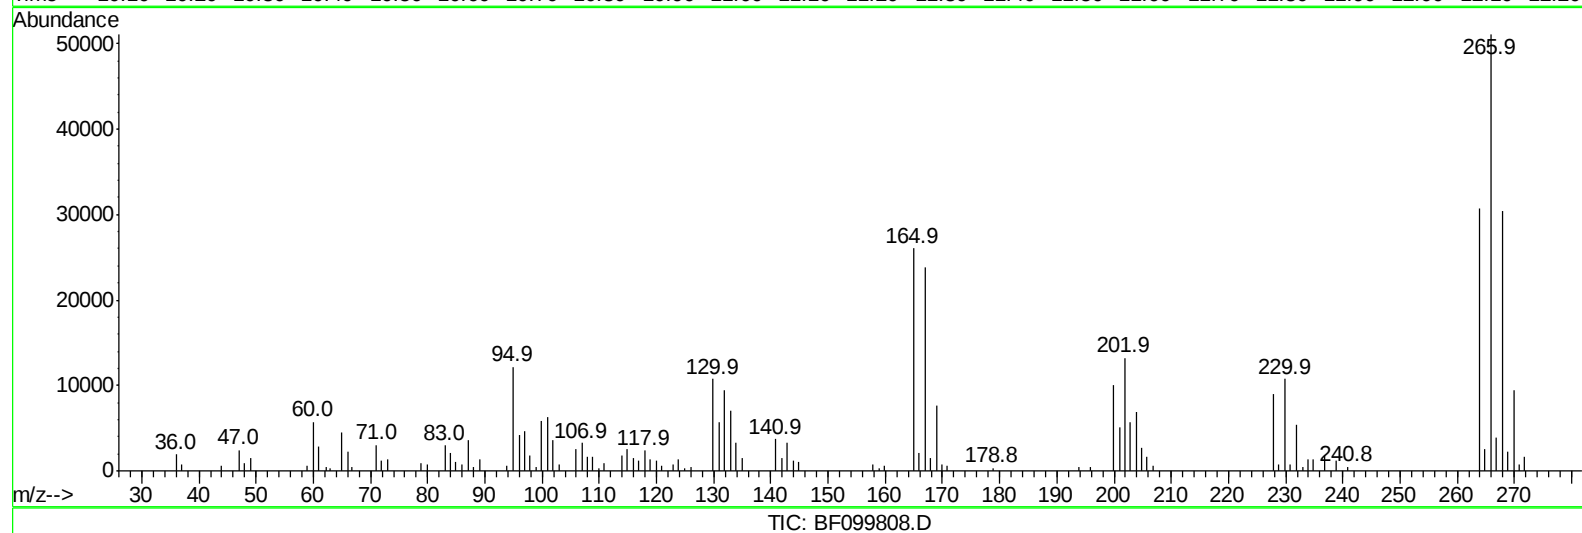


Data Path : Z:\HPCHEM1\BNA F\DATA\BF102517\
Data File : BF099808.D
Acq On : 25 Oct 2017 12:37
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 26 04:39:07 2017
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF102317.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Oct 25 17:02:52 2017
Response via : Initial Calibration

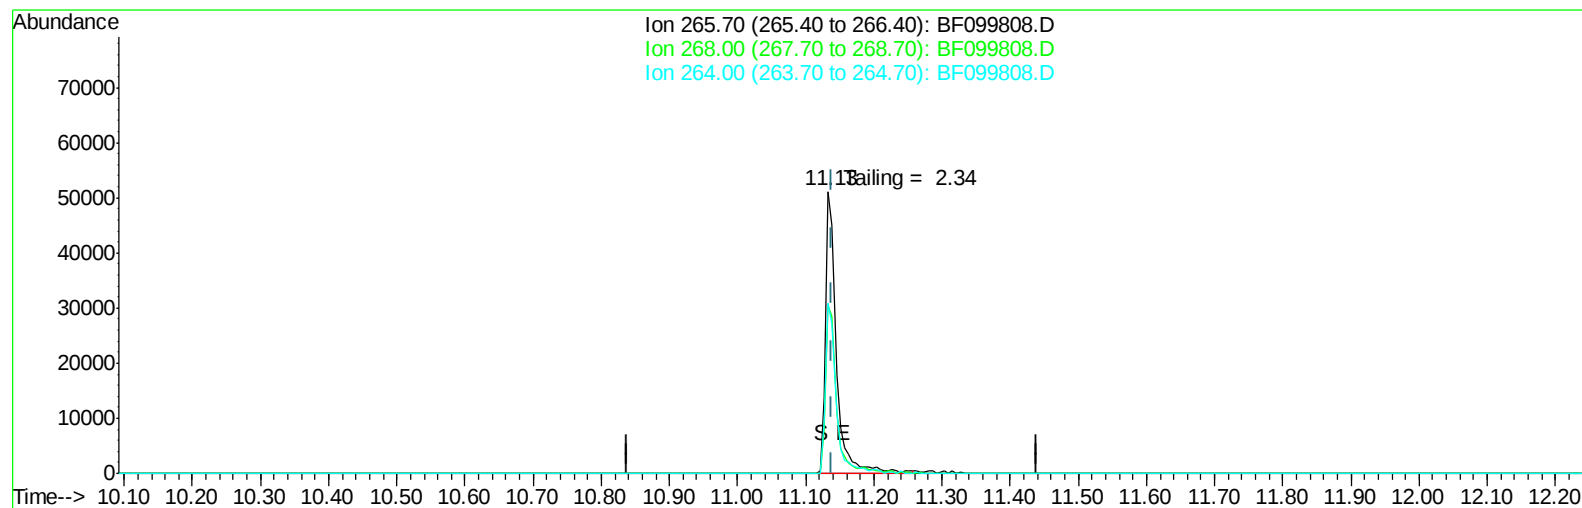

TIC: BF099808.D

(69) Pentachlorophenol (C)



11.133min (-0.006) 103051.08ng

response 55488

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	59.66
264.00	61.90	60.24
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA F\DATA\BF102517\
 Data File : BF099808.D
 Acq On : 25 Oct 2017 12:37
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 26 04:39:07 2017
 Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF102317.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Oct 25 17:02:52 2017
 Response via : Initial Calibration

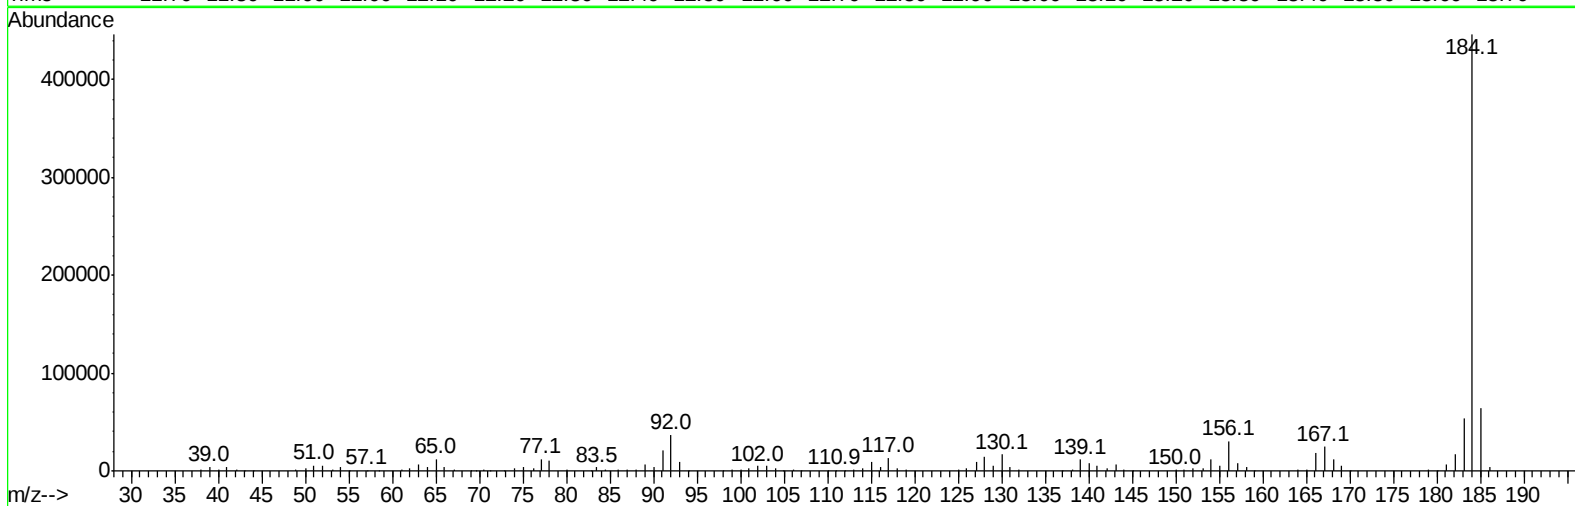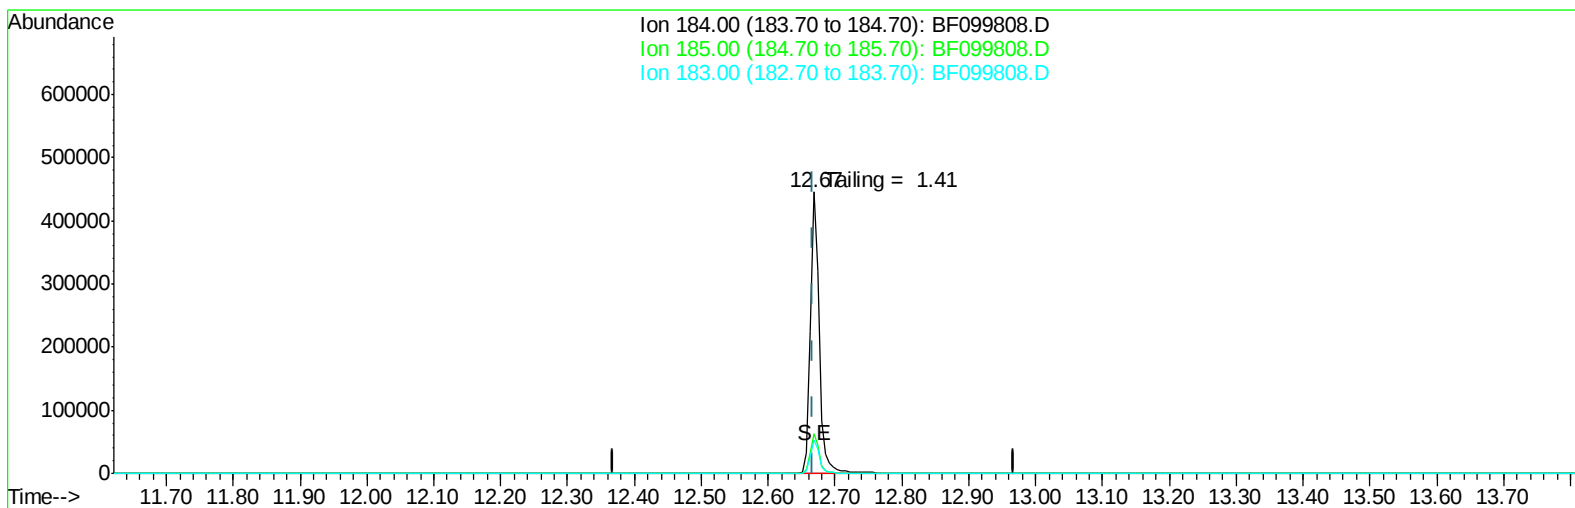

TIC: BF099808.D

(76) Benzidine

12.668min (-0.000) 0.00ng

response 422469

Ion	Exp%	Act%
184.00	100	100
185.00	15.70	14.29
183.00	11.60	11.93
0.00	0.00	0.00