
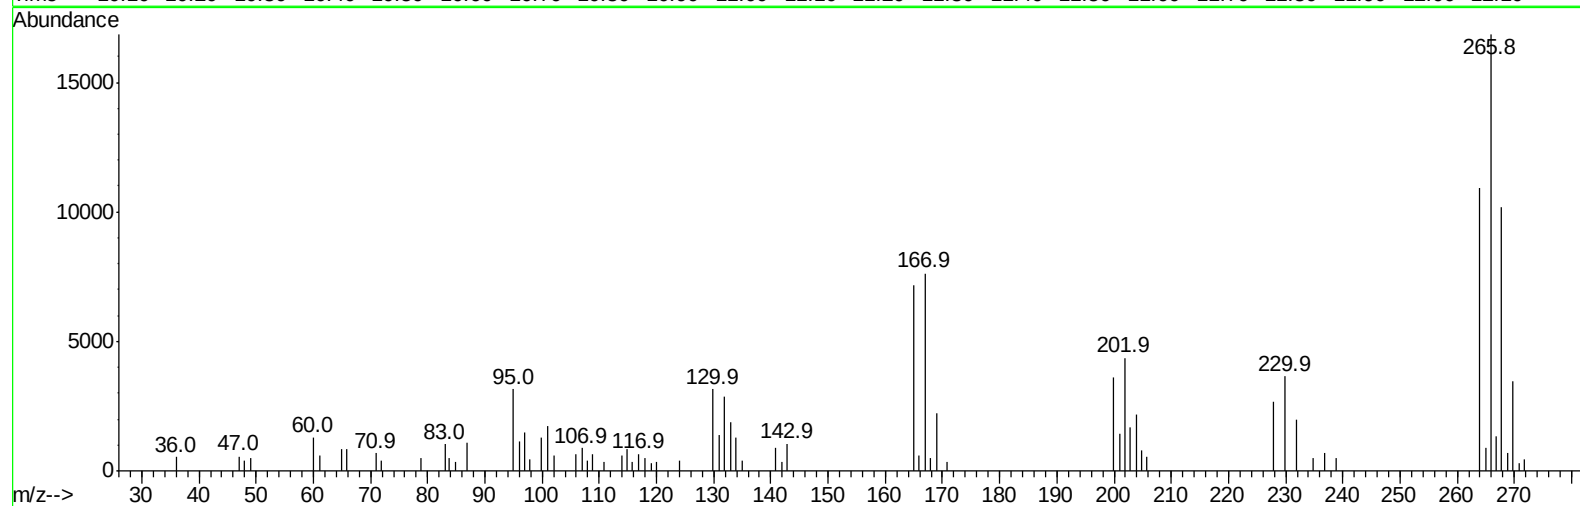


Data Path : Z:\HPCHEM1\BNA F\DATA\BF102517\
Data File : BF099833.D
Acq On : 26 Oct 2017 1:26
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 26 04:40:27 2017
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF102317.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Oct 25 17:02:52 2017
Response via : Initial Calibration

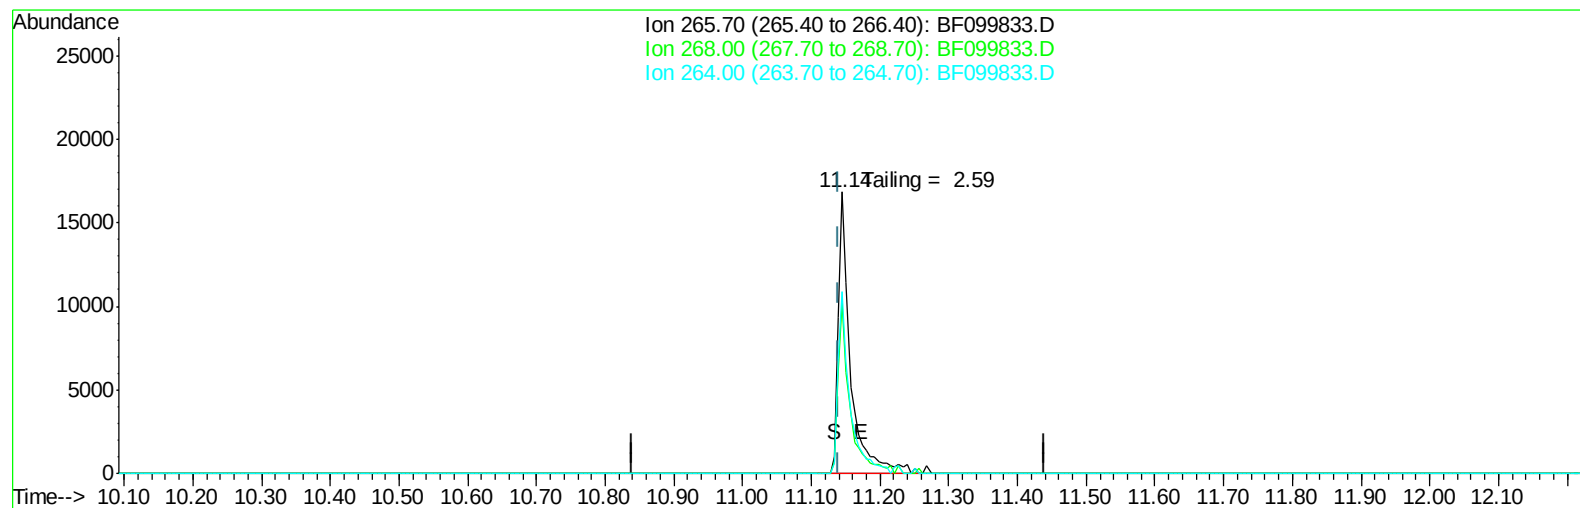

TIC: BF099833.D

(69) Pentachlorophenol (C)



11.145min (+0.006) 0.00ng

response 20310

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	60.37
264.00	61.90	64.68
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA F\DATA\BF102517\
Data File : BF099833.D
Acq On : 26 Oct 2017 1:26
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 26 04:40:27 2017
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF102317.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Oct 25 17:02:52 2017
Response via : Initial Calibration

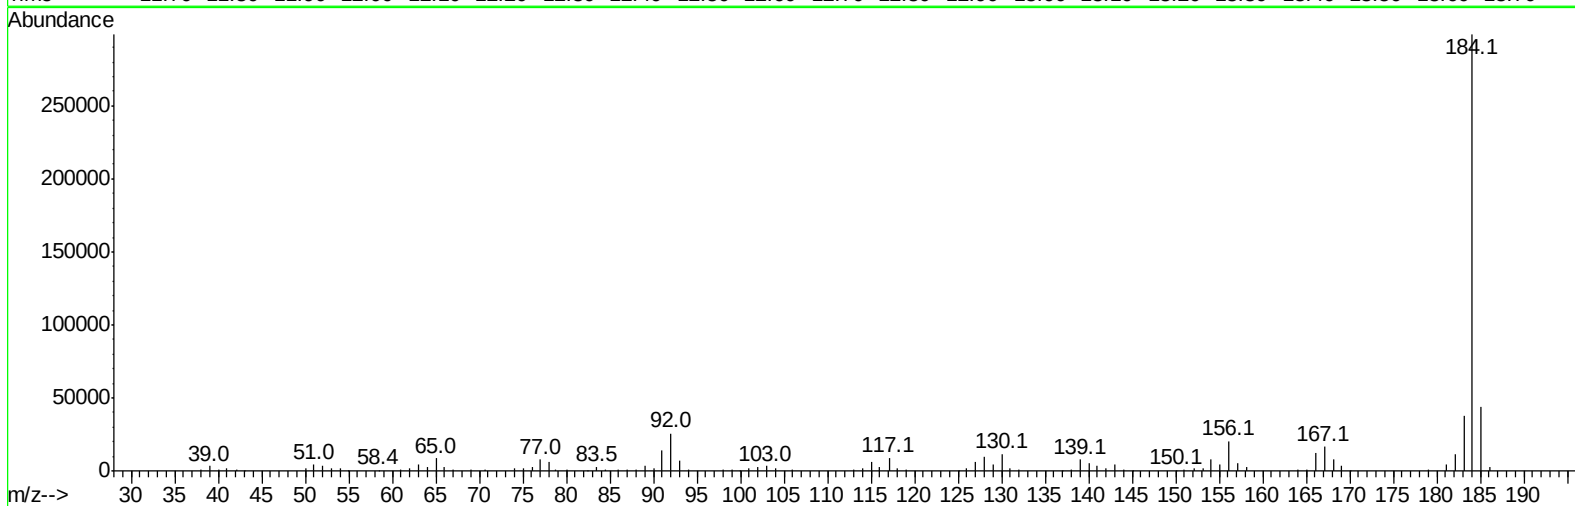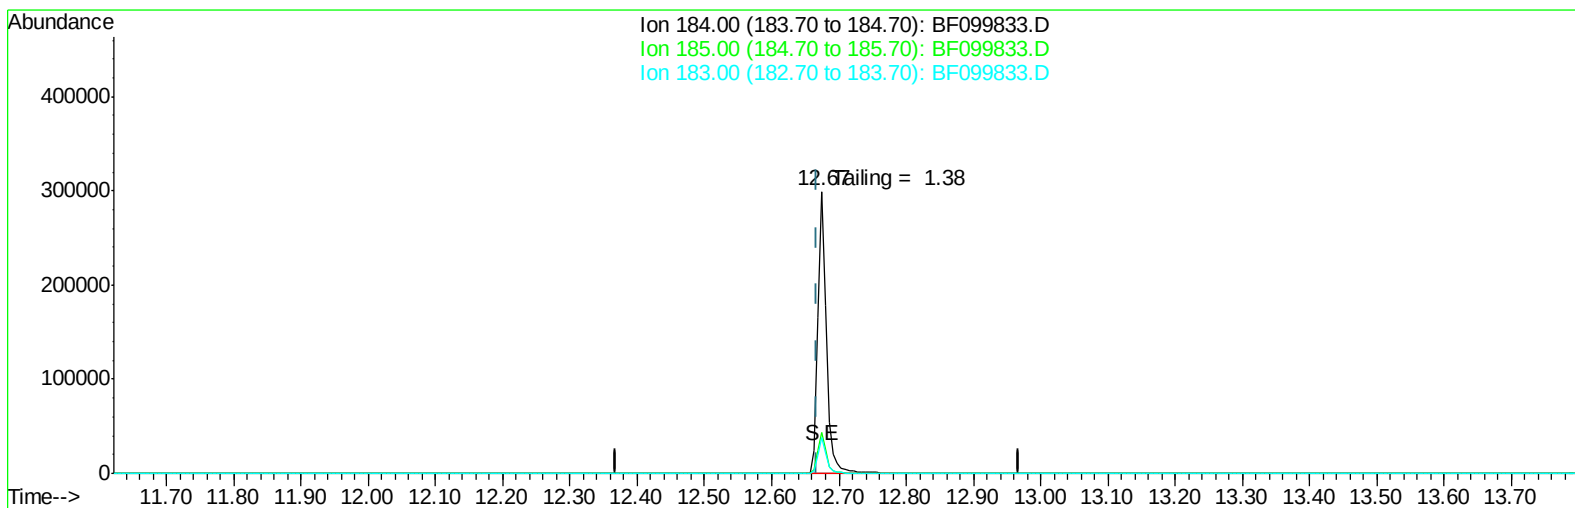

TIC: BF099833.D

(76) Benzidine

12.674min (+0.006) 26465.00ng

response 275612

Ion	Exp%	Act%
184.00	100	100
185.00	15.70	14.65
183.00	11.60	12.54
0.00	0.00	0.00