

Data Path : Z:\HPCHEM1\BNA F\DATA\BF102517\
 Data File : BF099840.D
 Acq On : 26 Oct 2017 4:45
 Operator : SJ/JU
 Sample : I6024-25
 Misc :
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 TWP-02

Quant Time: Oct 26 05:18:43 2017
 Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF102317.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Oct 25 17:02:52 2017
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	6.79	152	68601	20.00	ng	0.00
21) Naphthalene-d8	8.07	136	280191	20.00	ng	0.00
38) Acenaphthene-d10	9.83	164	124055	20.00	ng	0.00
63) Phenanthrene-d10	11.33	188	220008	20.00	ng	0.00
75) Chrysene-d12	13.98	240	184999	20.00	ng	0.00
86) Perylene-d12	15.45	264	158672	20.00	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.41	112	192244	44.00	ng	0.00
7) Phenol-d6	6.43	99	143445	27.69	ng	0.00
23) Nitrobenzene-d5	7.36	82	407358	93.60	ng	0.00
41) 2,4,6-Tribromophenol	10.63	330	101936	90.17	ng	0.00
44) 2-Fluorobiphenyl	9.16	172	809312	100.65	ng	0.00
78) Terphenyl-d14	12.92	244	748893	88.47	ng	0.00
Target Compounds						
49) Dimethylphthalate	9.55	163	91114	9.275	ng	99

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA F\DATA\BF102517\
Data File : BF099840.D
Acq On : 26 Oct 2017 4:45
Operator : SJ/JU
Sample : I6024-25
Misc :
ALS Vial : 30 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
TWP-02

Quant Time: Oct 26 05:18:43 2017
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF102317.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Oct 25 17:02:52 2017
Response via : Initial Calibration

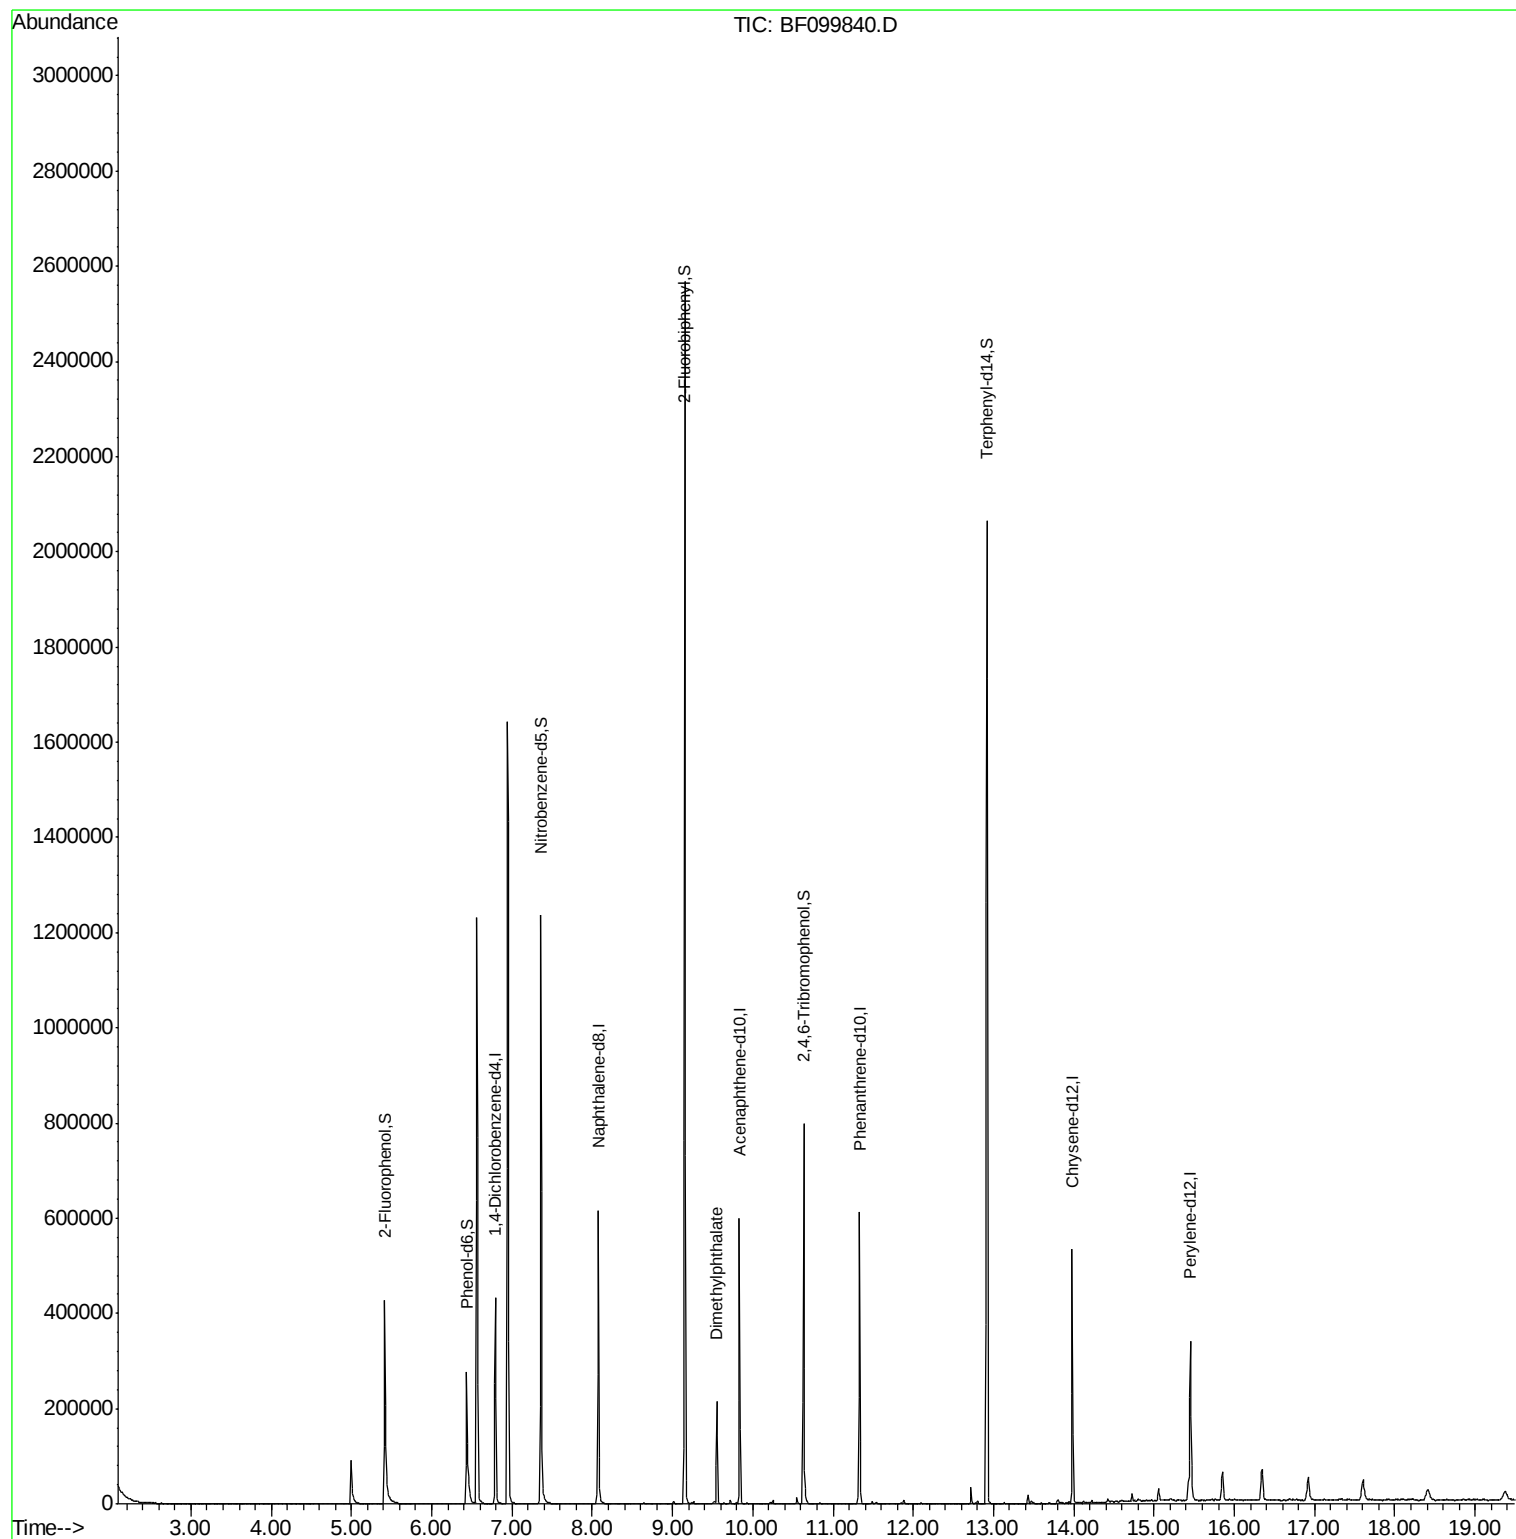




#1



1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 6.79 min Scan# 800
Delta R.T. 0.00 min
Lab File: BF099840.D
Acq: 26 Oct 2017 4:45

Instrument :
BNA_F
ClientSampleId :
TWP-02

Tot Ion:152 Resp: 68601
Ion Ratio Lower Upper
152 100
150 157.6 124.6 186.8
115 56.6 50.1 75.1

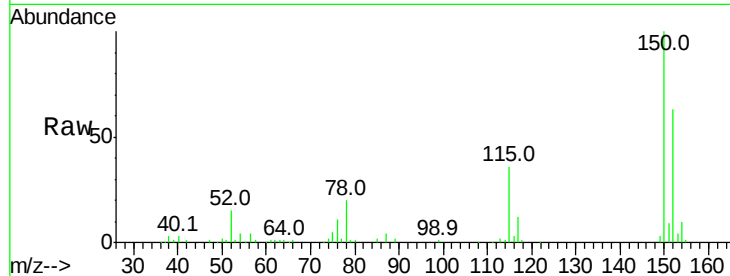


Abundance Ion 152.00 (151.70 to 152.70): E
Ion 150.00 (149.70 to 150.70): E
Ion 115.00 (114.70 to 115.70): E

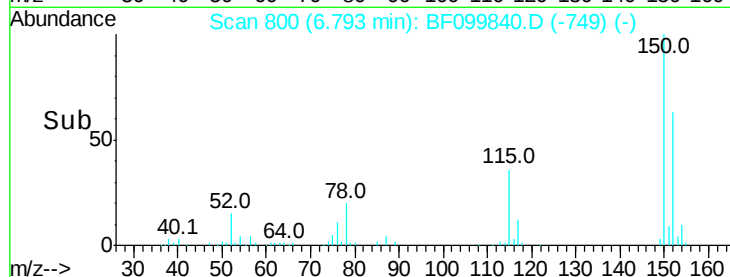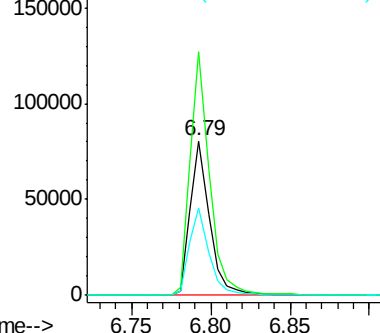



#5

2-Fluorophenol
Concen: 43.996 ng
RT: 5.41 min Scan# 565
Delta R.T. 0.00 min
Lab File: BF099840.D
Acq: 26 Oct 2017 4:45

Tgt Ion:112 Resp: 192244
Ion Ratio Lower Upper
112 100
64 52.2 47.9 71.9
63 23.9 23.7 35.5

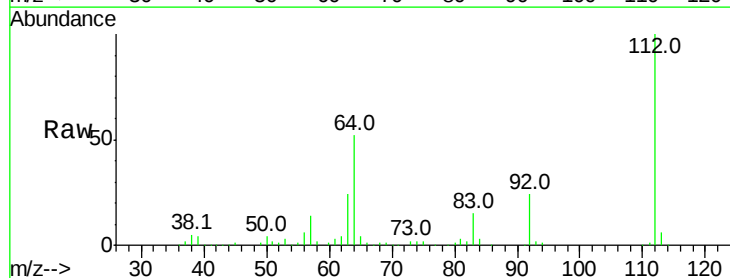

Abundance Ion 112.00 (111.70 to 112.70): E
Ion 64.00 (63.70 to 64.70): BF0
Ion 63.00 (62.70 to 63.70): BF0

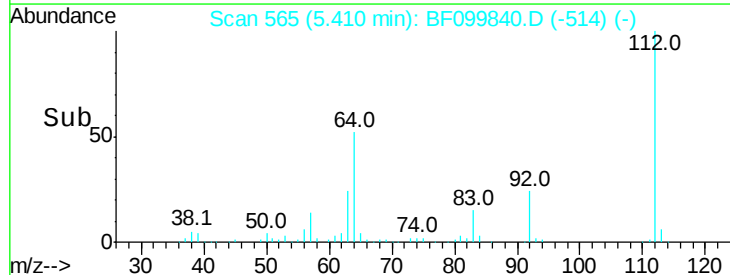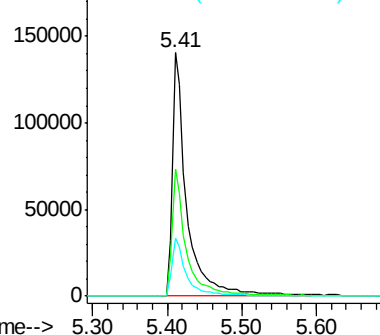



#7

Phenol-d6

Concen: 27.686 ng

RT: 6.43 min Scan# 739

Delta R.T. -0.01 min

Lab File: BF099840.D

Acq: 26 Oct 2017 4:45

Instrument :

BNA_F

ClientSampleId :

TWP-02


Tot Ion: 99 Resp: 143445

Ion Ratio Lower Upper

99 100

42 13.7 14.5 21.7#



71 28.5 25.4 38.0

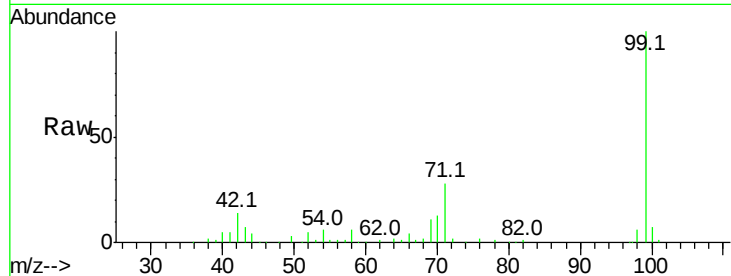

Abundance Ion 99.00 (98.70 to 99.70): BF0

Ion 42.00 (41.70 to 42.70): BF0

Ion 71.00 (70.70 to 71.70): BF0

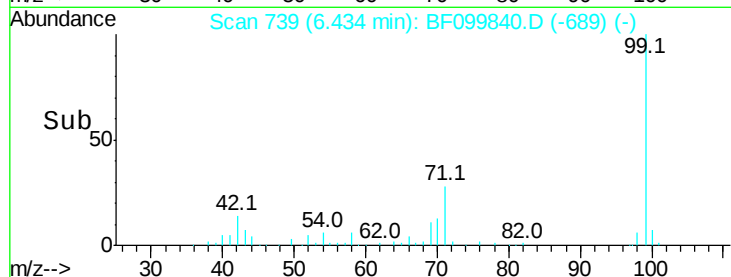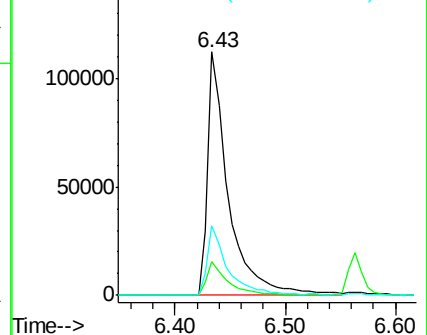

#21

Naphthalene-d8

Concen: 20.000 ng

RT: 8.07 min Scan# 1018

Delta R.T. -0.01 min

Lab File: BF099840.D

Acq: 26 Oct 2017 4:45

Tgt Ion: 136 Resp: 280191


Ion Ratio Lower Upper

136 100

137 10.9 8.9 13.3

54 6.7 6.6 9.8

68 5.7 5.0 7.4


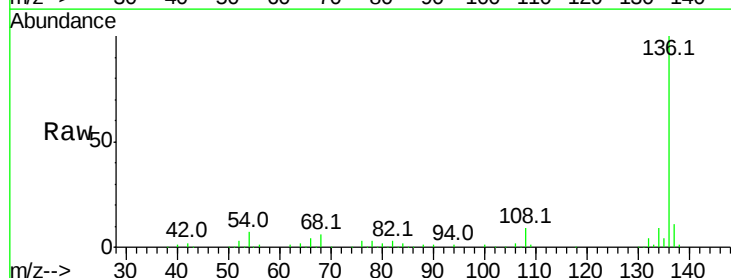



Abundance Ion 136.00 (135.70 to 136.70): E

Ion 137.00 (136.70 to 137.70): E

Ion 54.00 (53.70 to 54.70): BF0

Ion 68.00 (67.70 to 68.70): BF0

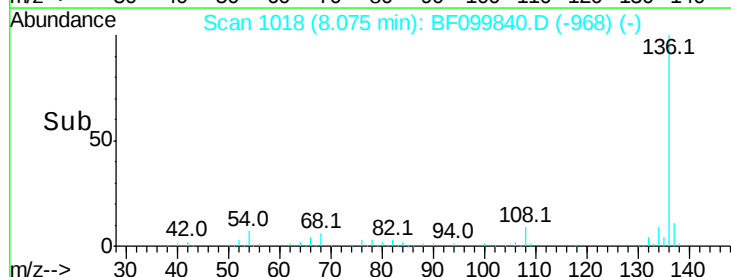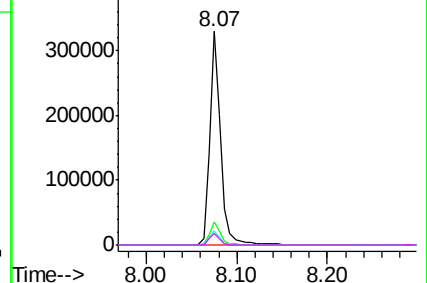

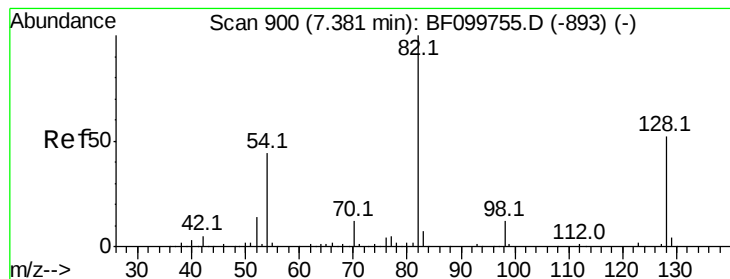

#23

Nitrobenzene-d5

Concen: 93.600 ng

RT: 7.36 min Scan# 897

Delta R.T. -0.01 min

Lab File: BF099840.D

Acq: 26 Oct 2017 4:45

Instrument :

BNA_F

ClientSampleId :

TWP-02


Tot Ion: 82 Resp: 407358

Ion Ratio Lower Upper




82 100

128 50.0 36.1 54.1

54 43.5 41.4 62.2

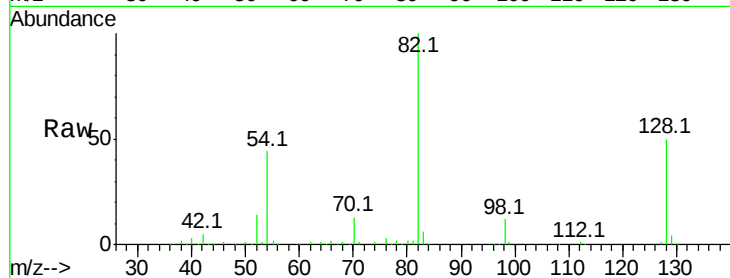

Abundance Ion 82.00 (81.70 to 82.70): BF0
Ion 128.00 (127.70 to 128.70): E
Ion 54.00 (53.70 to 54.70): BF0

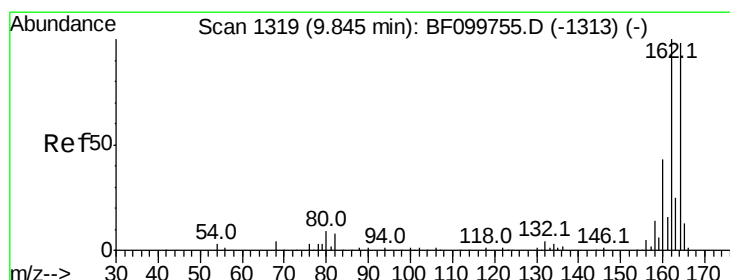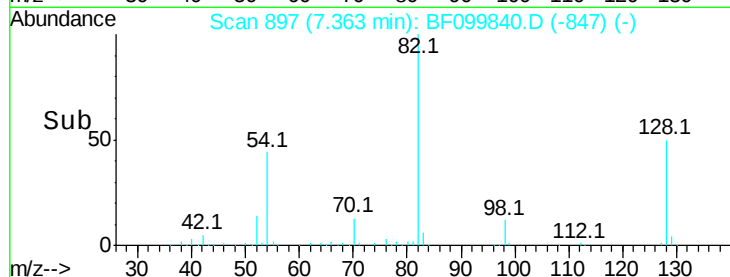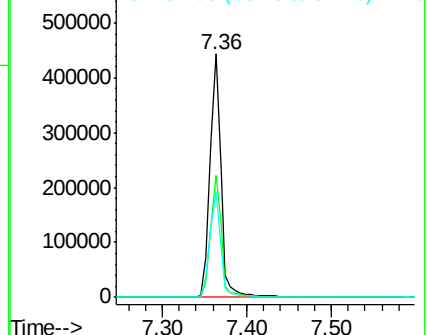

#38

Acenaphthene-d10

Concen: 20.000 ng

RT: 9.83 min Scan# 1317

Delta R.T. -0.01 min

Lab File: BF099840.D

Acq: 26 Oct 2017 4:45


Tgt Ion:164 Resp: 124055

Ion Ratio Lower Upper



164 100

162 105.2 86.1 129.1

160 44.8 38.3 57.5

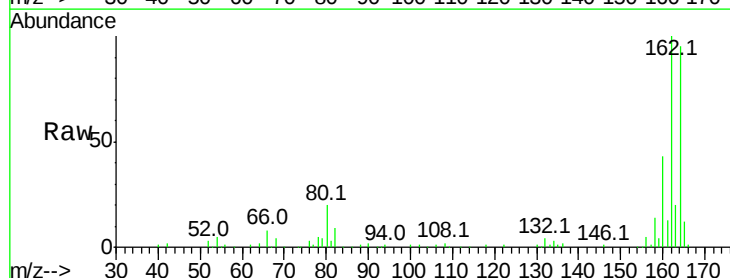

Abundance Ion 164.00 (163.70 to 164.70): E
Ion 162.00 (161.70 to 162.70): E
Ion 160.00 (159.70 to 160.70): E

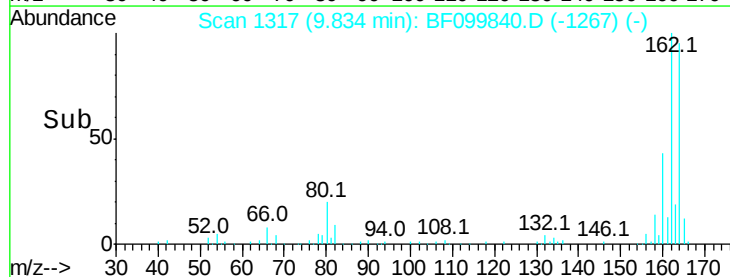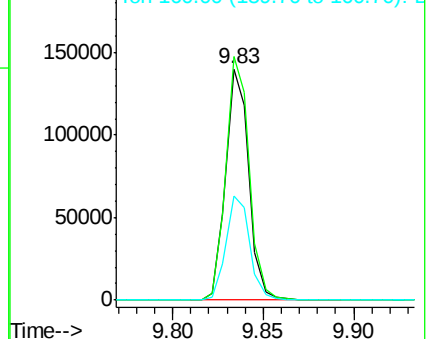







#41
 2,4,6-Tribromophenol
 Concen: 90.166 ng
 RT: 10.63 min Scan# 1453
 Delta R.T. 0.00 min
 Lab File: BF099840.D
 Acq: 26 Oct 2017 4:45

Instrument :
 BNA_F
 ClientSampleId :
 TWP-02

Tot Ion	Ratio	Lower	Upper
330	100		
332	95.9	77.0	115.6
141	36.0	29.9	44.9

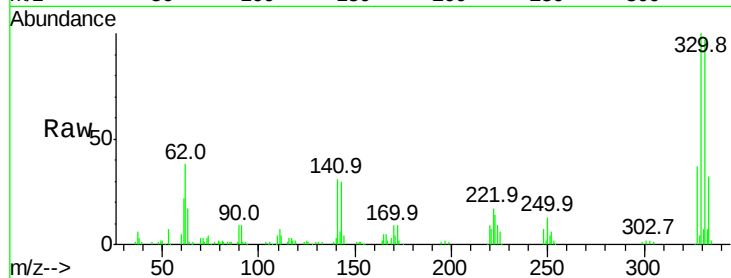


Abundance Ion 329.80 (329.50 to 330.50): E
 Ion 331.80 (331.50 to 332.50): E
 Ion 141.00 (140.70 to 141.70): E

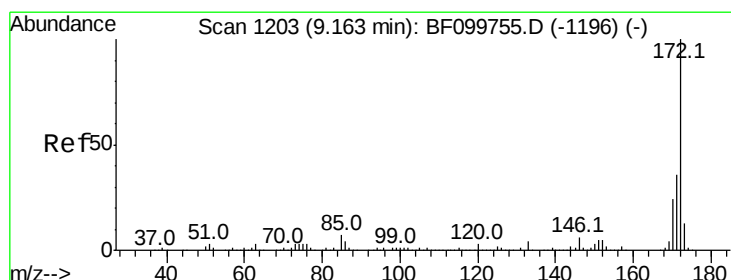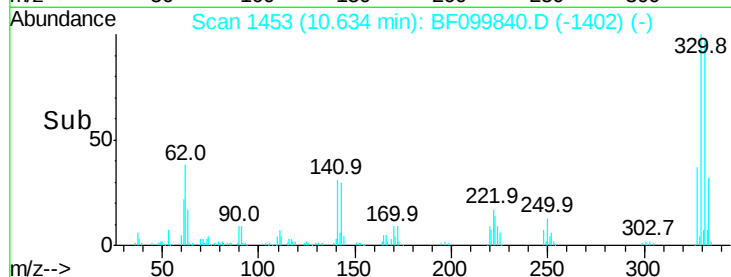
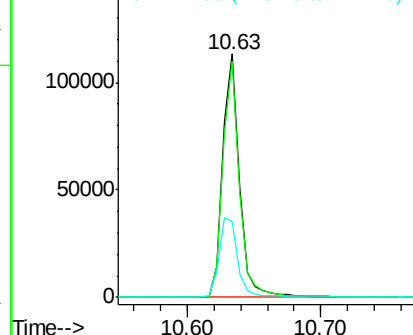



#44
 2-Fluorobiphenyl
 Concen: 100.652 ng
 RT: 9.16 min Scan# 1202
 Delta R.T. 0.00 min
 Lab File: BF099840.D
 Acq: 26 Oct 2017 4:45

Tgt Ion	Ratio	Lower	Upper
172	100		
171	35.8	29.7	44.5
170	23.6	19.6	29.4

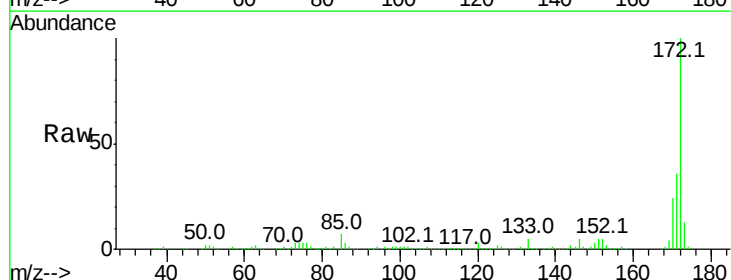

Abundance Ion 172.00 (171.70 to 172.70): E
 Ion 171.00 (170.70 to 171.70): E
 Ion 170.00 (169.70 to 170.70): E

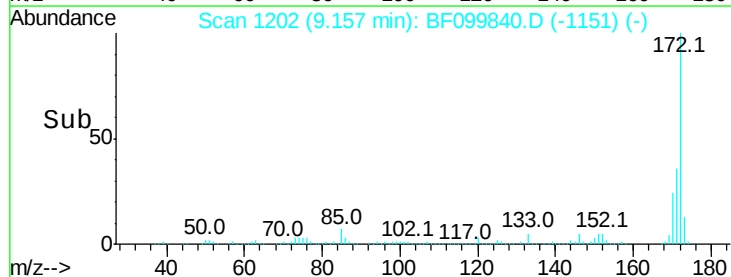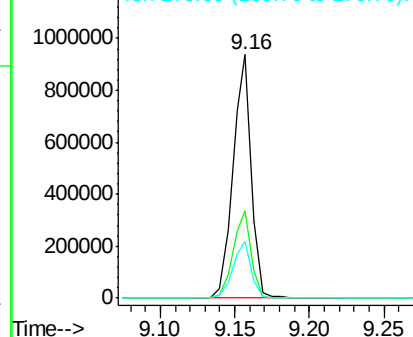

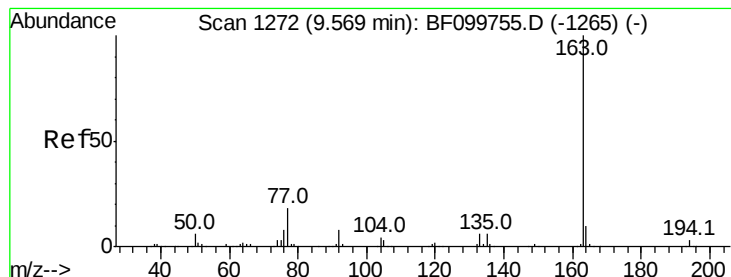

#49

Dimethylphthalate

Concen: 9.275 ng

RT: 9.55 min Scan# 1269

Delta R.T. -0.01 min

Lab File: BF099840.D

Acq: 26 Oct 2017 4:45

Instrument :

BNA_F

ClientSampled :

TWP-02


Tot Ion:163 Resp: 91114

Ion Ratio Lower Upper

163 100

194 4.0 2.7 4.1




164 10.0 8.2 12.2

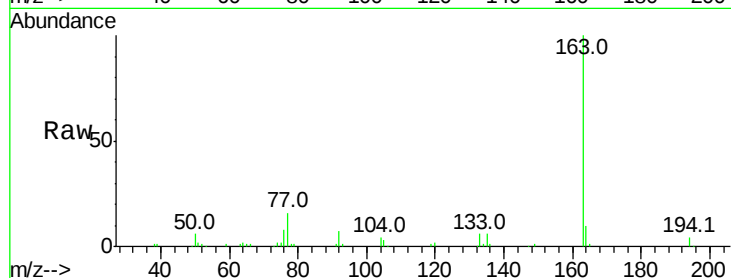

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

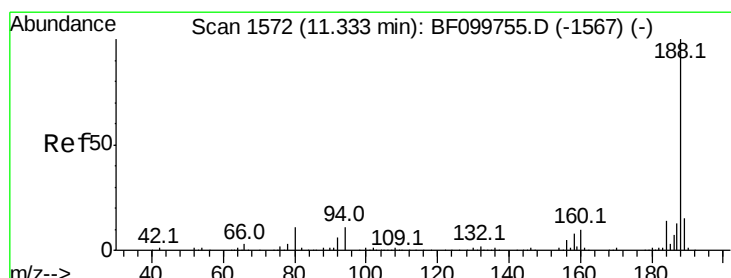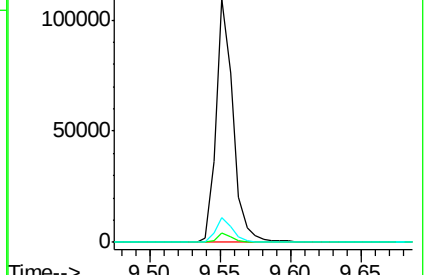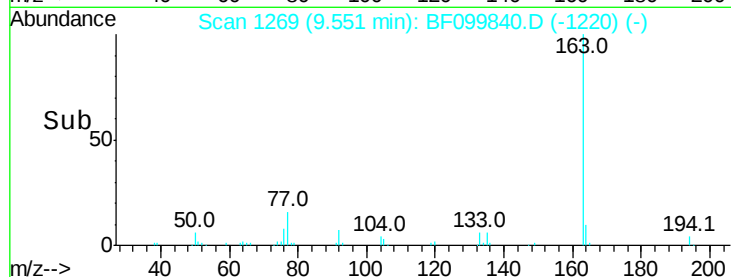

#63

Phenanthrene-d10

Concen: 20.000 ng

RT: 11.33 min Scan# 1571

Delta R.T. 0.00 min

Lab File: BF099840.D

Acq: 26 Oct 2017 4:45


Tgt Ion:188 Resp: 220008

Ion Ratio Lower Upper

188 100

94 10.5 8.5 12.7



80 11.3 9.2 13.8

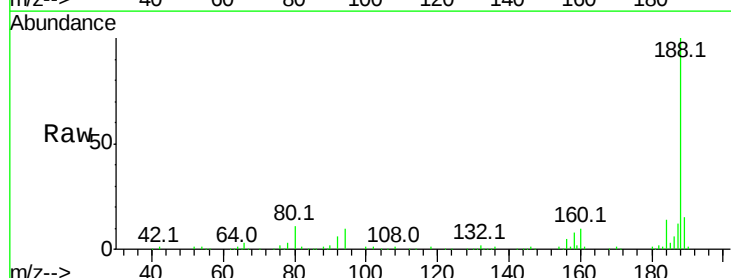


Abundance Ion 188.00 (187.70 to 188.70): E

Ion 94.00 (93.70 to 94.70): BF0

Ion 80.00 (79.70 to 80.70): BF0



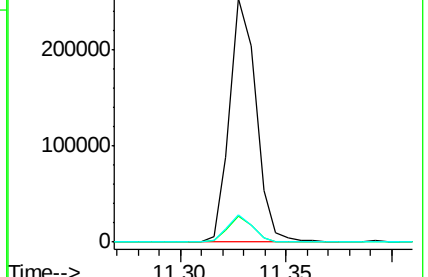
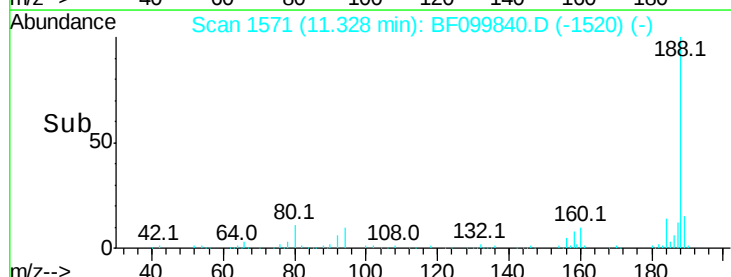


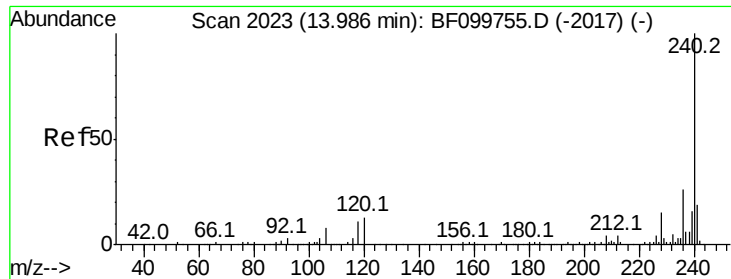

#75
 Chrysene-d12
 Concen: 20.000 ng
 RT: 13.98 min Scan# 2022
 Delta R.T. 0.00 min
 Lab File: BF099840.D
 Acq: 26 Oct 2017 4:45




Instrument :
 BNA_F
 ClientSampleID :
 TWP-02


Tot Ion:240 Resp: 184999
 Ion Ratio Lower Upper
 240 100
 120 15.2 9.5 14.3#
 236 25.4 20.7 31.1

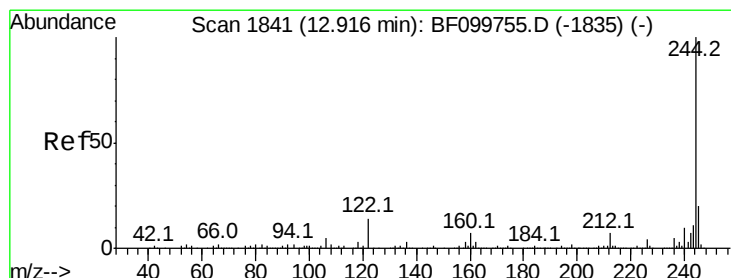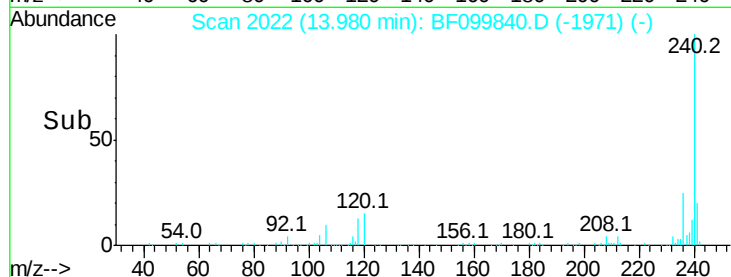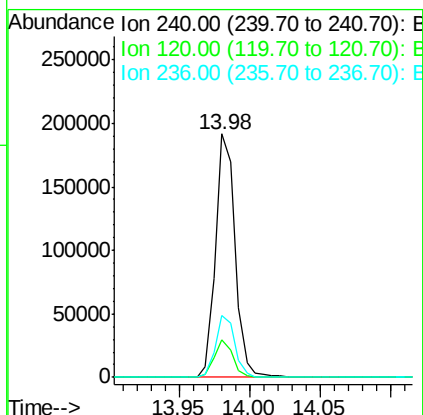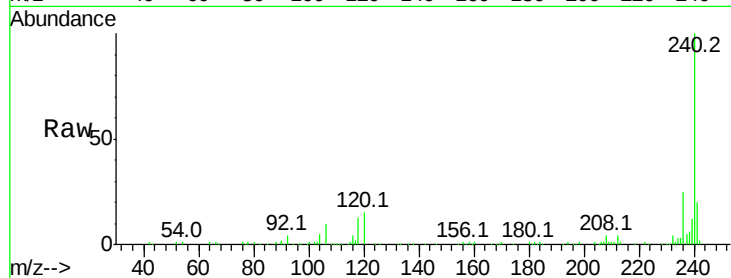

#78
 Terphenyl-d14
 Concen: 88.466 ng
 RT: 12.92 min Scan# 1841
 Delta R.T. 0.00 min
 Lab File: BF099840.D
 Acq: 26 Oct 2017 4:45

Tgt Ion:244 Resp: 748893
 Ion Ratio Lower Upper
 244 100
 212 6.7 5.4 8.0
 122 14.0 11.0 16.4

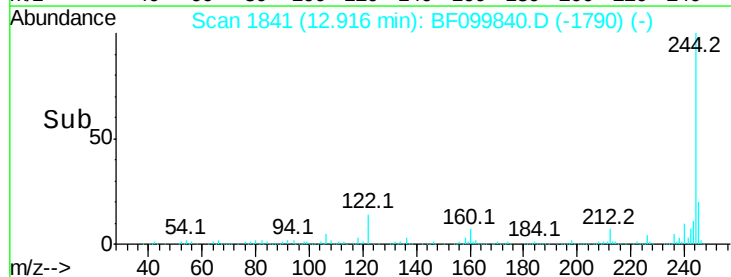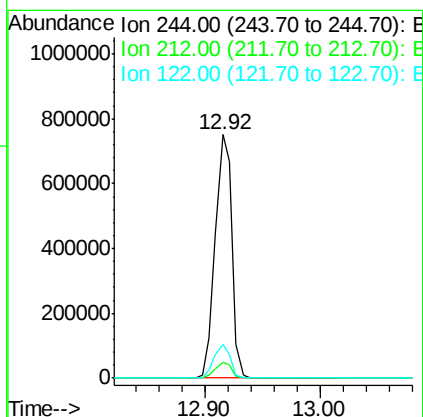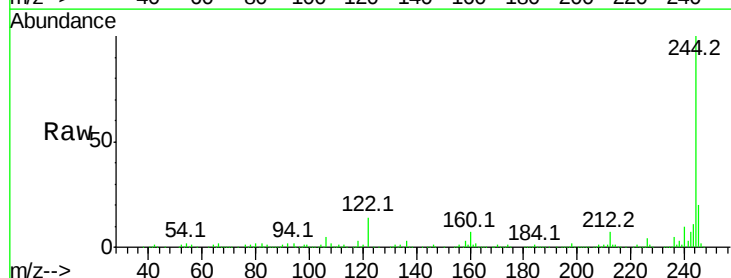


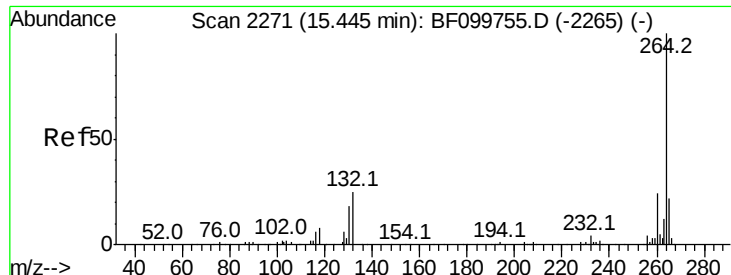

#86
 Pervlene-d12
 Concen: 20.000 ng
 RT: 15.45 min Scan# 2272
 Delta R.T. 0.01 min
 Lab File: BF099840.D
 Acq: 26 Oct 2017 4:45

Instrument :
 BNA_F
 ClientSampleId :
 TWP-02

Tot Ion	Ratio	Lower	Upper
264	100		
260	23.1	19.2	28.8
265	21.0	17.5	26.3

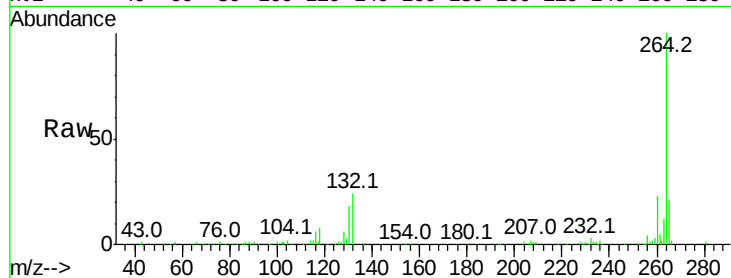

Abundance Ion 264.00 (263.70 to 264.70): E
 Ion 260.00 (259.70 to 260.70): E
 Ion 265.00 (264.70 to 265.70): E

