


Data Path : Z:\HPCHEM1\BNA F\Data\BF102517\
 Data File : BF099808.D
 Acq On : 25 Oct 2017 12:37
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF102317.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Oct 25 17:02:52 2017

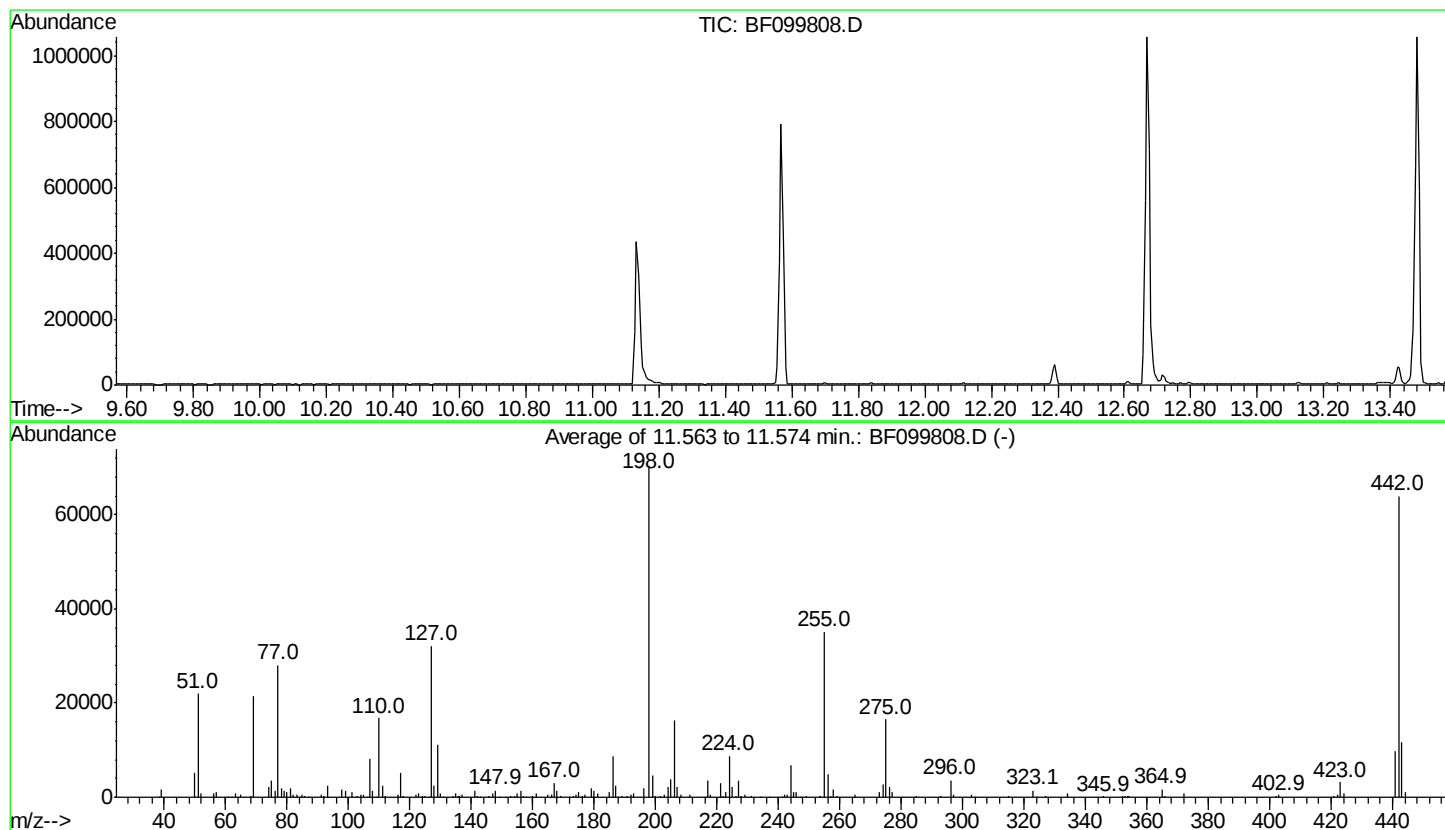

AutoFind: Scans 1611, 1612, 1613; Background Corrected with Scan 1606

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	31.1	21920	PASS
68	69	0.00	2	1.5	314	PASS
69	198	0.00	100	30.6	21532	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	45.7	32189	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	70394	PASS
199	198	5	9	6.5	4544	PASS
275	198	10	60	23.4	16497	PASS
365	198	1	100	2.5	1750	PASS
441	442	0.01	24	15.2	9739	PASS
442	198	50	100	90.8	63941	PASS
443	442	15	24	18.2	11648	PASS