


Data Path : Z:\HPCHEM1\BNA F\Data\BF102517\
 Data File : BF099833.D
 Acq On : 26 Oct 2017 1:26
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF102317.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Oct 25 17:02:52 2017

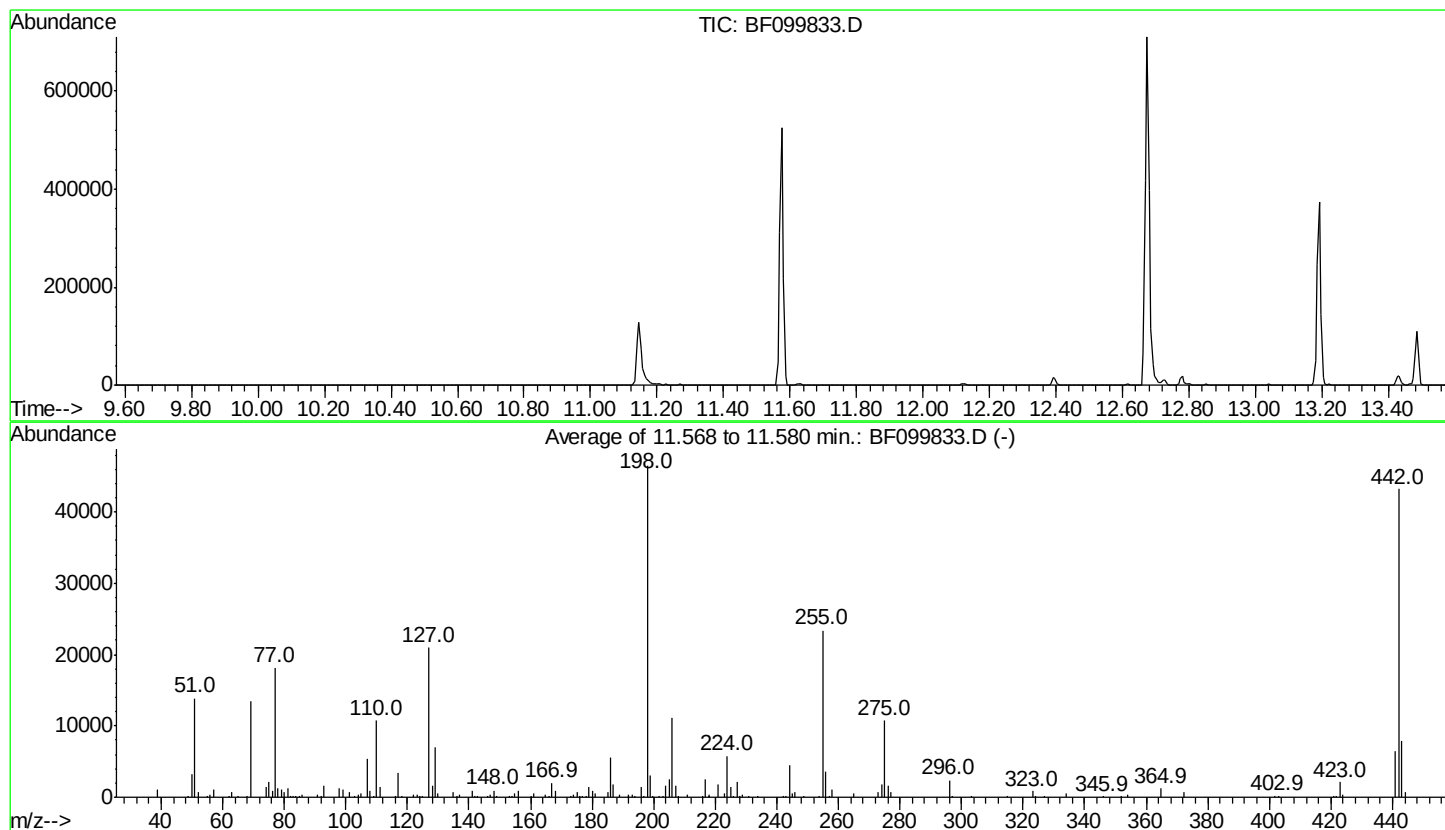

AutoFind: Scans 1612, 1613, 1614; Background Corrected with Scan 1607

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	29.9	13910	PASS
68	69	0.00	2	1.2	160	PASS
69	198	0.00	100	28.9	13455	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	45.1	20962	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	46493	PASS
199	198	5	9	6.6	3051	PASS
275	198	10	60	23.1	10731	PASS
365	198	1	100	2.5	1183	PASS
441	442	0.01	24	15.1	6539	PASS
442	198	50	100	92.9	43181	PASS
443	442	15	24	18.5	7993	PASS