
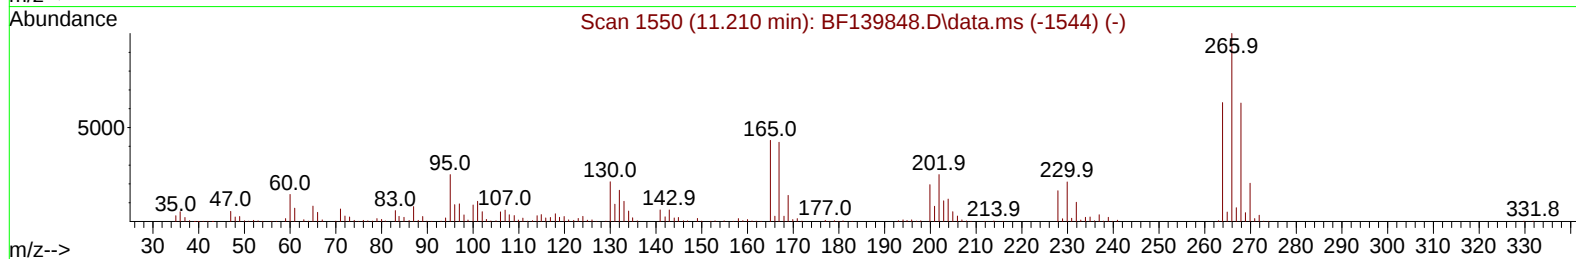
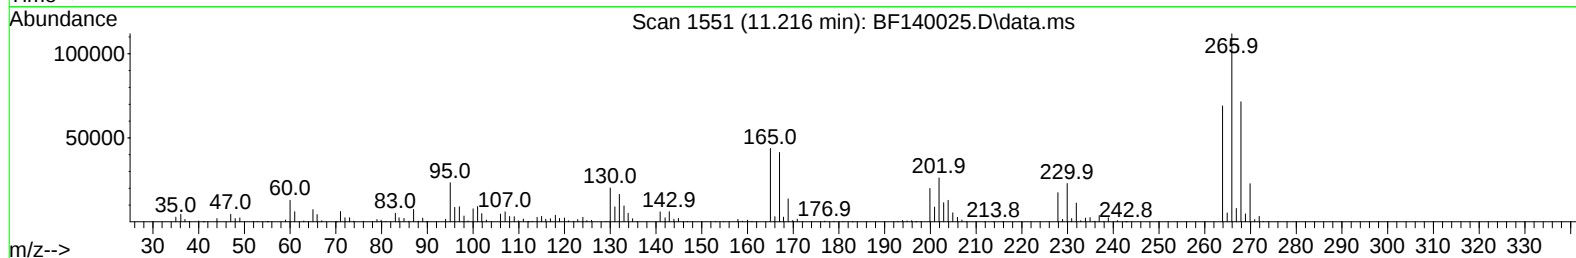


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF102524\
Data File : BF140025.D
Acq On : 25 Oct 2024 09:20
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 25 11:33:54 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF101824.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Oct 18 15:07:50 2024
Response via : Initial Calibration

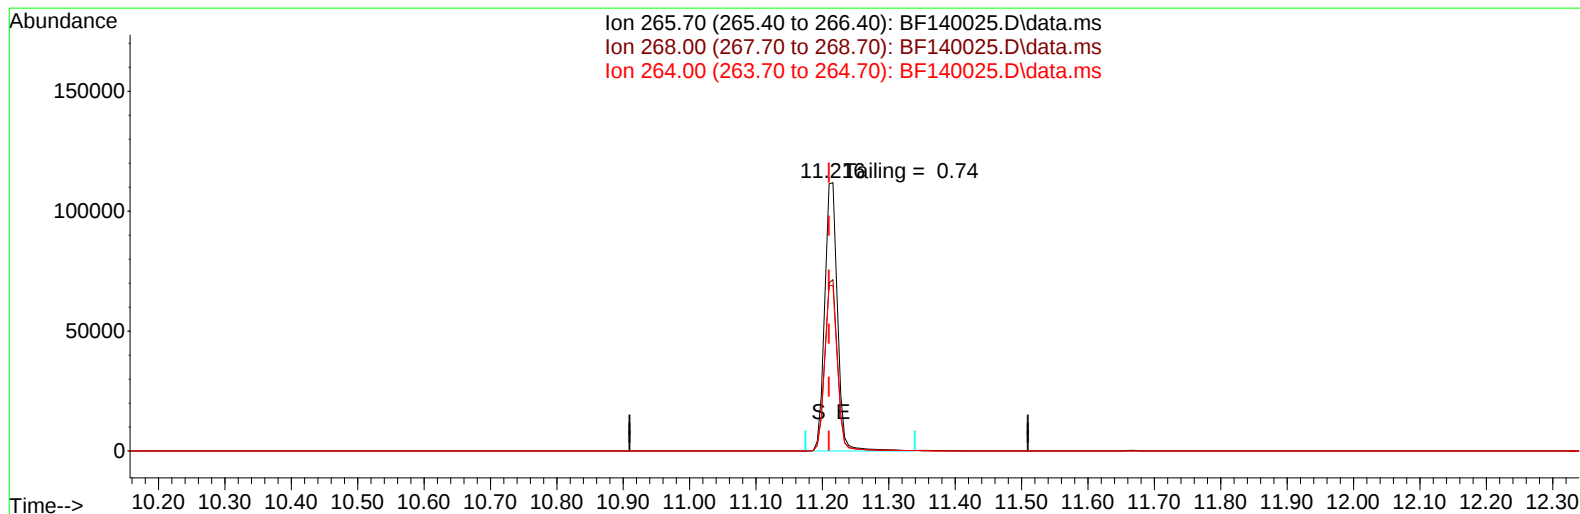

TIC: BF140025.D\data.ms

(70) Pentachlorophenol (C)




11.216min (+ 0.006) 28094.47 ng

response 150535

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.00	63.89
264.00	63.20	61.67
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF102524\
Data File : BF140025.D
Acq On : 25 Oct 2024 09:20
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 25 11:33:54 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF101824.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Oct 18 15:07:50 2024
Response via : Initial Calibration

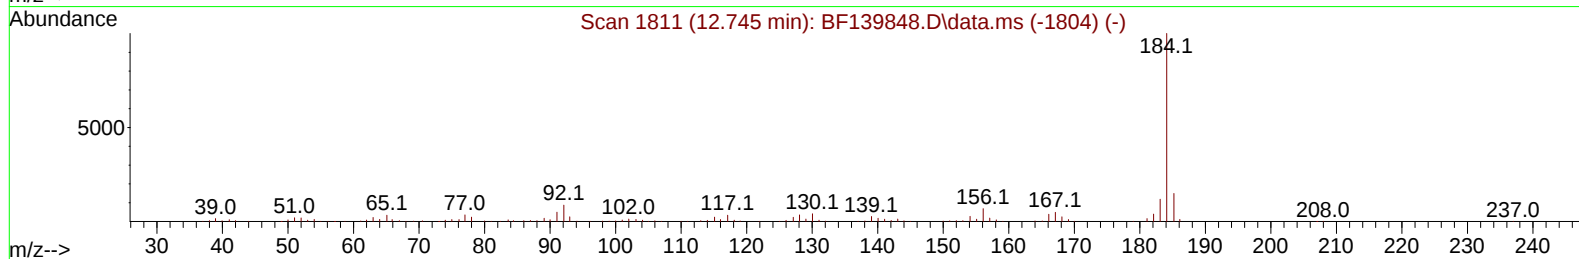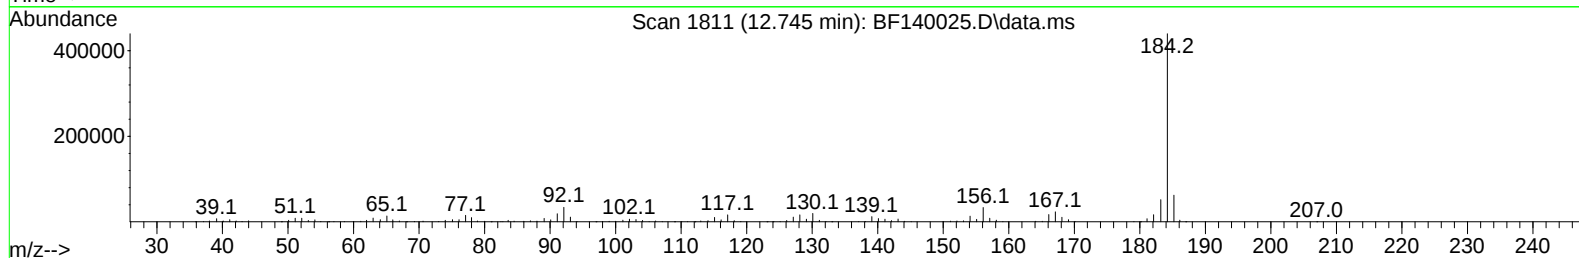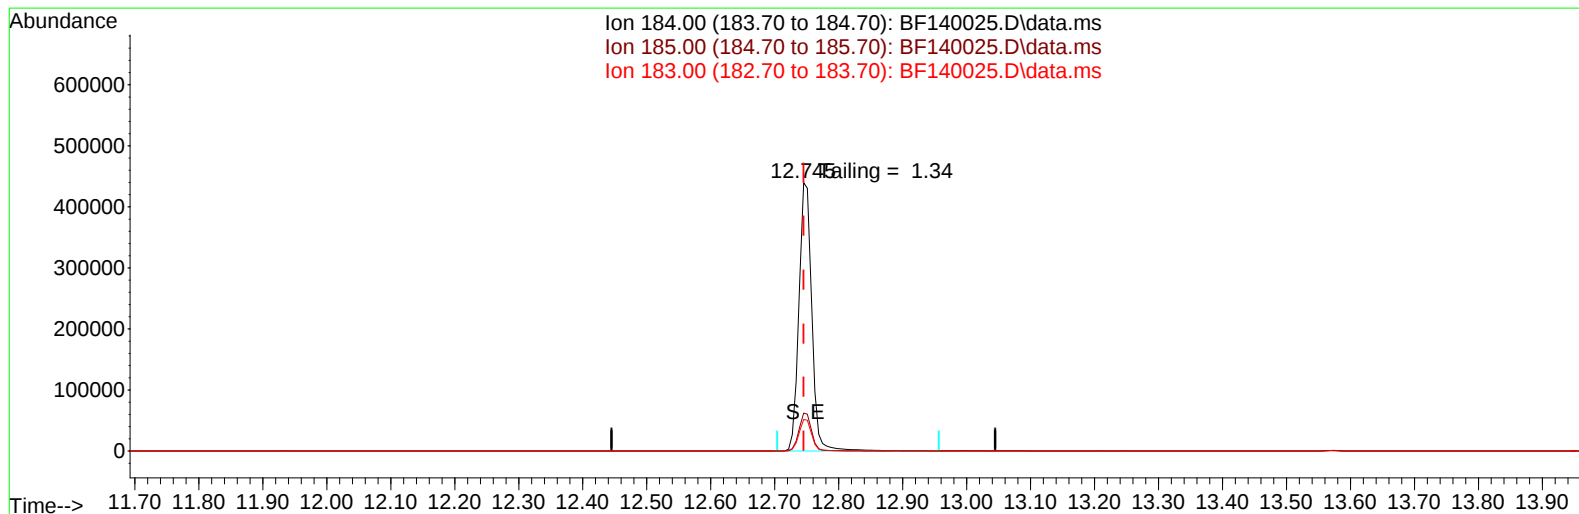

TIC: BF140025.D\data.ms

(77) Benzidine

12.745min (+ 0.000) 95286.91 ng

response 618902

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.00	14.14
183.00	11.80	11.79
0.00	0.00	0.00