

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF102524\
Data File : BF140027.D
Acq On : 25 Oct 2024 10:17
Operator : RC/JU
Sample : PB164366BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB164366BL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 3 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF101824.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF140027.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.516	575	582	587	rBV	1961536	2791707	82.79%	13.332%
2	6.510	744	751	756	rBV	1895818	2824593	83.76%	13.489%
3	6.887	810	815	820	rVB	512271	628194	18.63%	3.000%
4	7.445	903	910	916	rBV	1317671	1881701	55.80%	8.986%
5	8.169	1027	1033	1038	rBV	632671	817958	24.26%	3.906%
6	9.245	1209	1216	1221	rBV	2509293	3372215	100.00%	16.105%
7	9.922	1325	1331	1349	rVB	697216	934916	27.72%	4.465%
8	10.716	1459	1466	1490	rBV	1548363	2141061	63.49%	10.225%
9	11.410	1579	1584	1592	rBV	745702	945221	28.03%	4.514%
10	12.998	1848	1854	1859	rBV	2565487	3366471	99.83%	16.077%
11	14.051	2025	2033	2055	rBV	526110	728403	21.60%	3.479%
12	15.527	2278	2284	2298	rVB	288735	507072	15.04%	2.422%




Sum of corrected areas: 20939512

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF102524\
Data File : BF140027.D
Acq On : 25 Oct 2024 10:17
Operator : RC/JU
Sample : PB164366BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB164366BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF101824.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

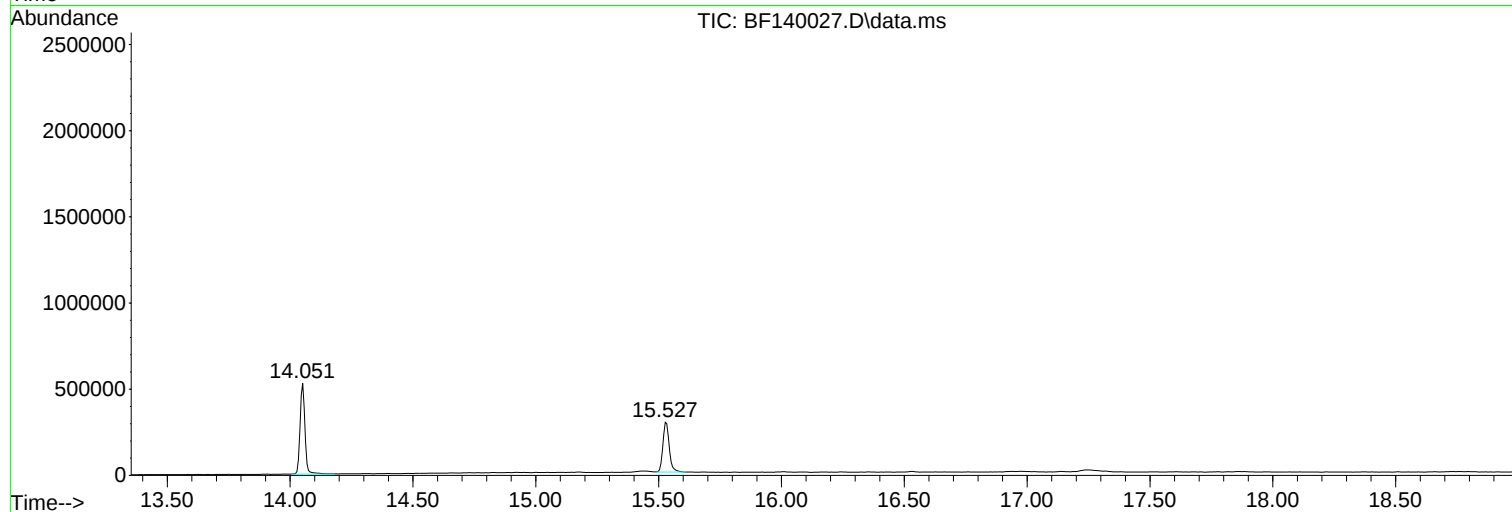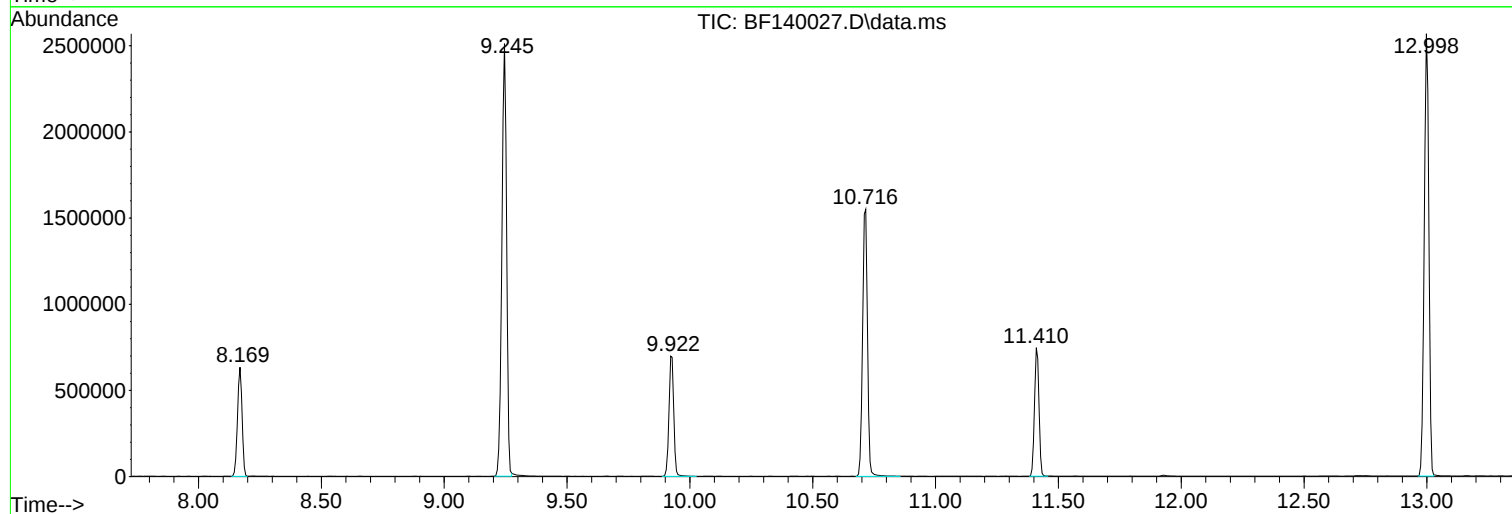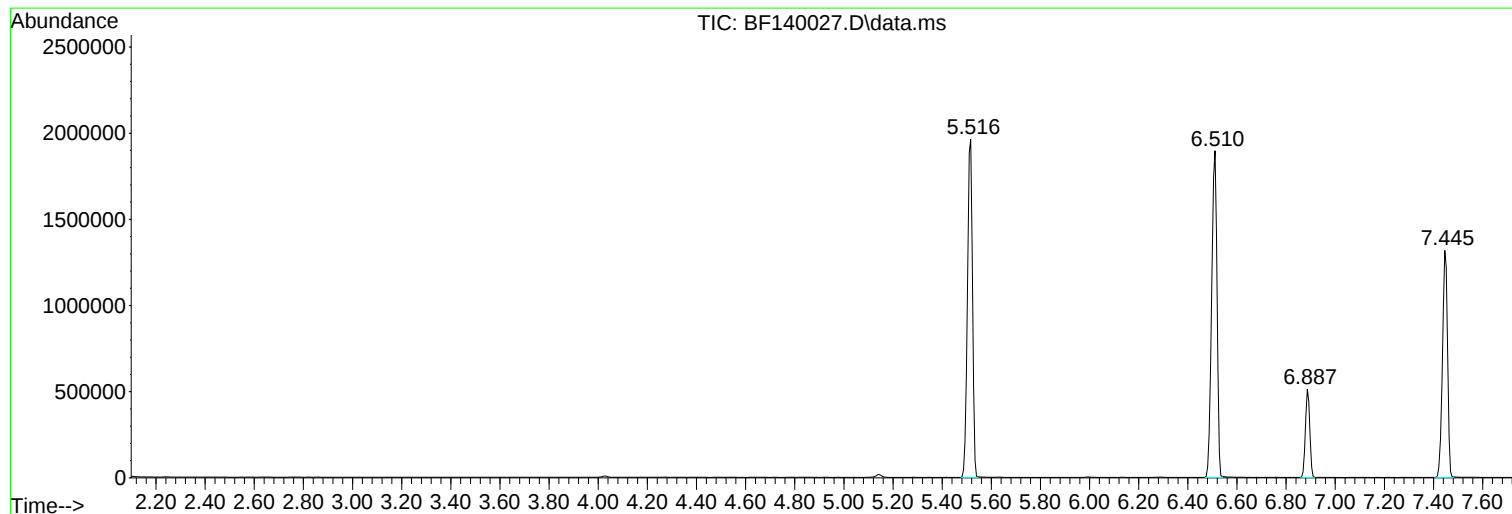

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF102524\
Data File : BF140027.D
Acq On : 25 Oct 2024 10:17
Operator : RC/JU
Sample : PB164366BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB164366BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF101824.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF102524\
Data File : BF140027.D
Acq On : 25 Oct 2024 10:17
Operator : RC/JU
Sample : PB164366BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB164366BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF101824.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------