
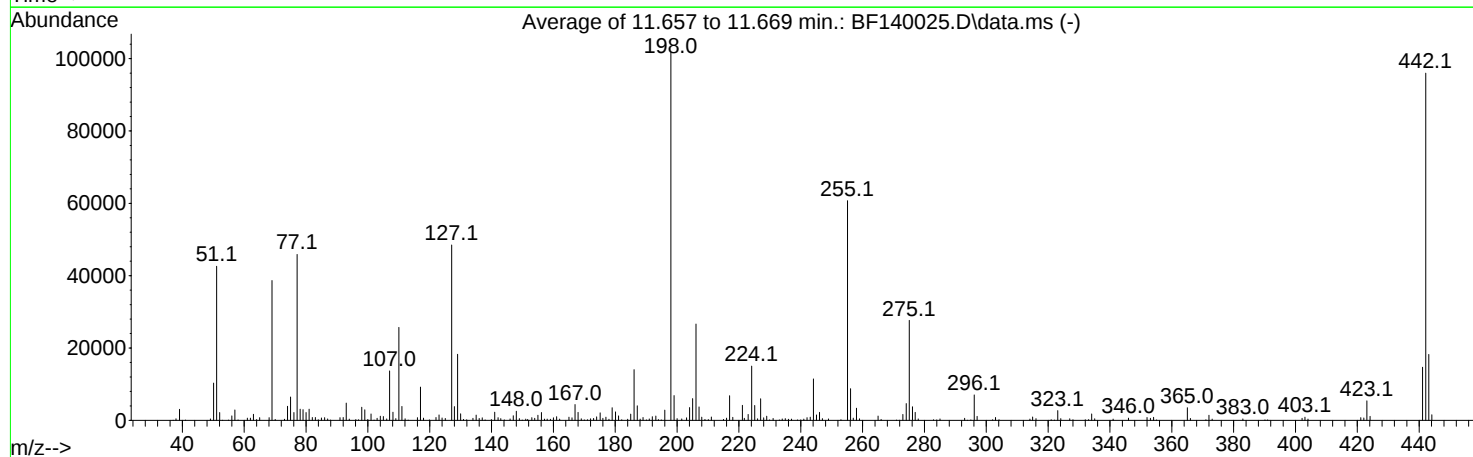


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF102524\
Data File : BF140025.D
Acq On : 25 Oct 2024 09:20
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF101824.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Fri Oct 18 15:07:50 2024

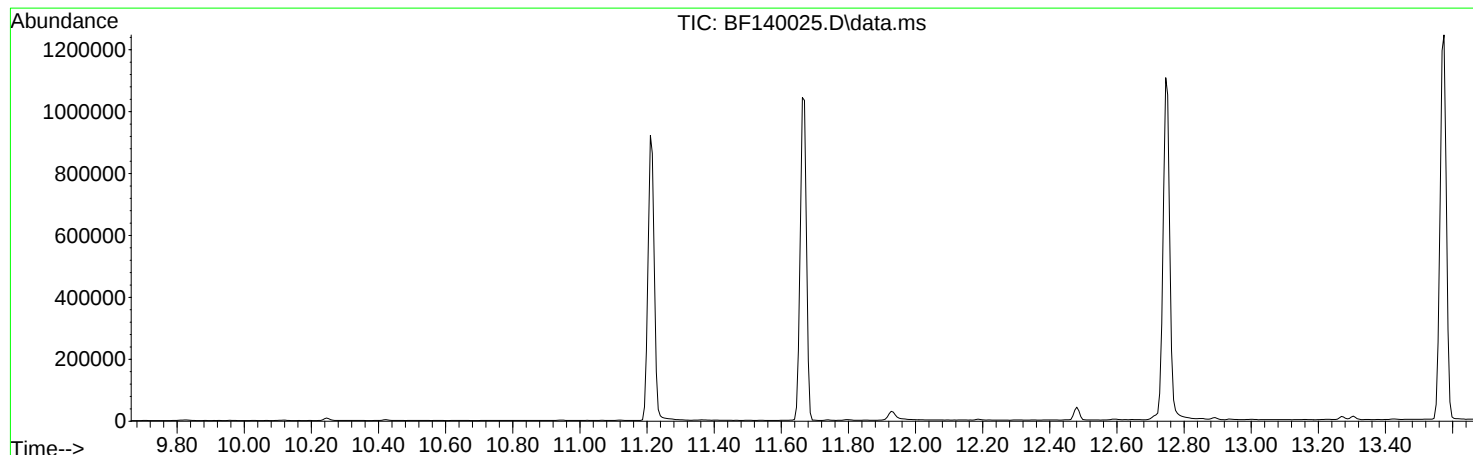

AutoFind: Scans 1626, 1627, 1628; Background Corrected with Scan 1620

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	41.9	42616	PASS
68	69	0.00	2	1.9	753	PASS
69	198	0.00	100	38.0	38659	PASS
70	69	0.00	2	0.7	252	PASS
127	198	10	80	47.7	48499	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	101691	PASS
199	198	5	9	6.7	6843	PASS
275	198	10	60	27.2	27645	PASS
365	198	1	100	3.4	3502	PASS
441	198	0.01	100	14.5	14703	PASS
442	442	50	100	100.0	95987	PASS
443	442	15	24	19.0	18231	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
10/25/2024	BNA_F	<u>BF140025.D</u>
Compound Name	Response	Retention Time
DDT	320982	13.575
DDD	6074	13.269
DDE	878	12.939
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
6952	327934	2.12

Instrument :
BNA_F
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF102524\
Data File : BF140025.D
Acq On : 25 Oct 2024 09:20
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Oct 25 11:33:54 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF101824.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Oct 18 15:07:50 2024
Response via : Initial Calibration

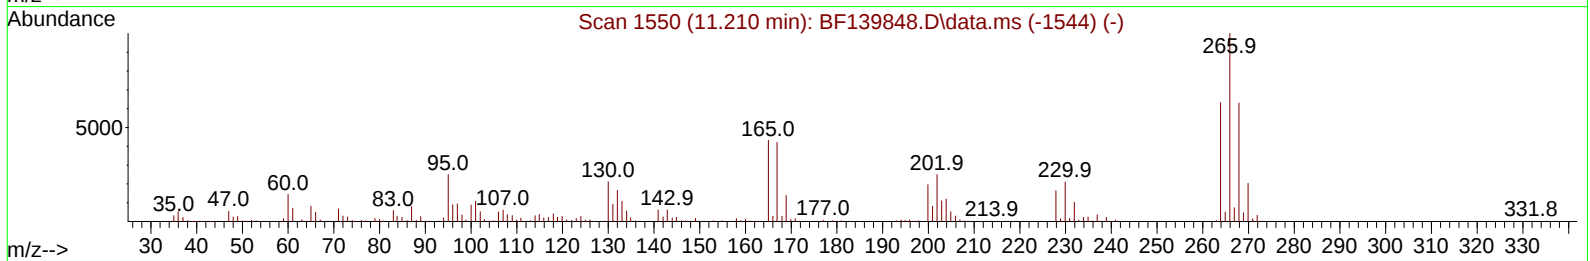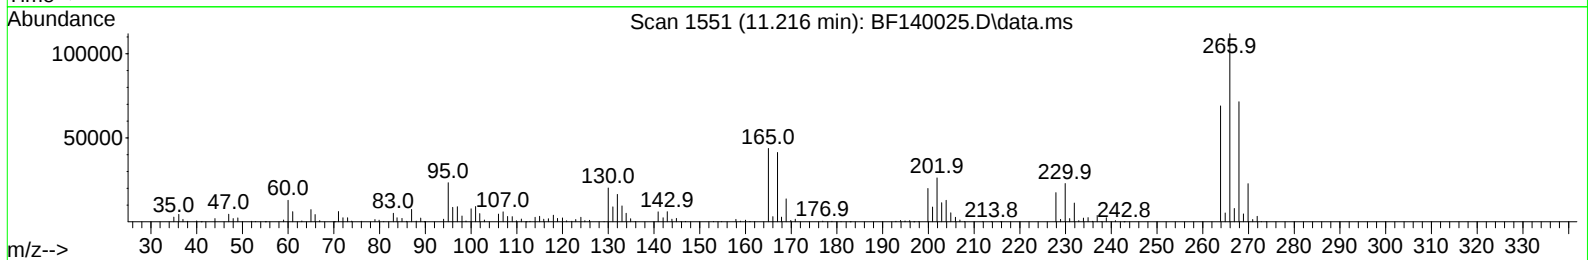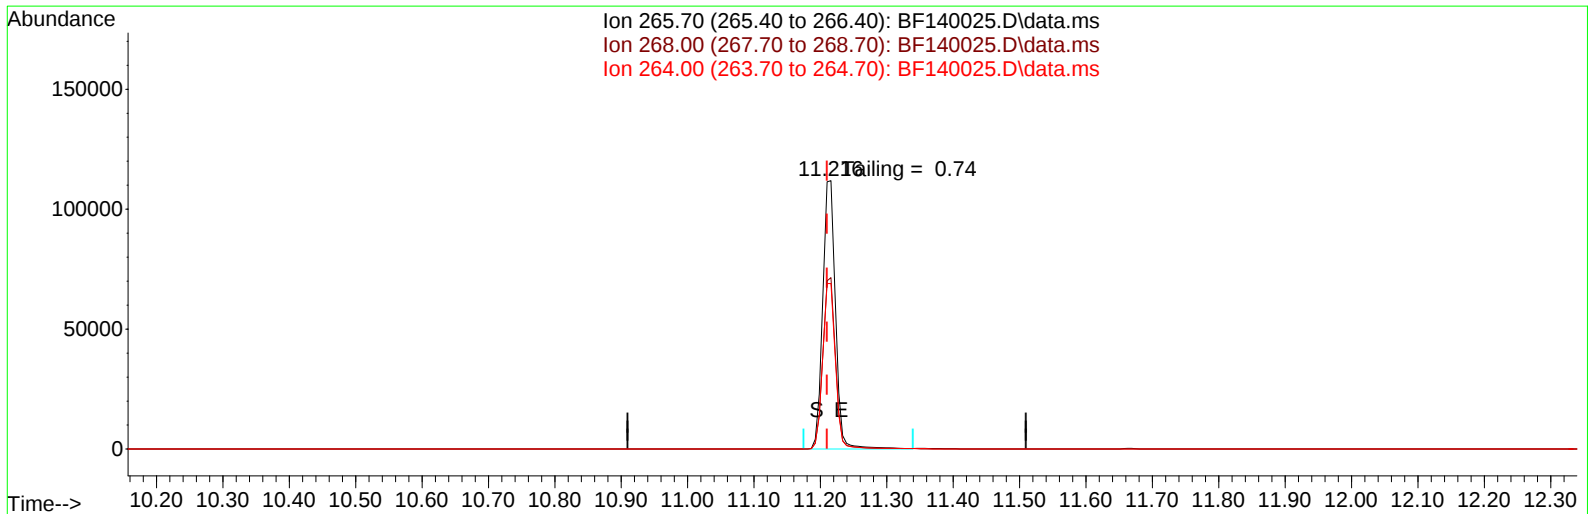

TIC: BF140025.D\data.ms

(70) Pentachlorophenol (C)

11.216min (+ 0.006) 28094.47 ng




response 150535

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.00	63.89
264.00	63.20	61.67
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF102524\
Data File : BF140025.D
Acq On : 25 Oct 2024 09:20
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Oct 25 11:33:54 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF101824.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Oct 18 15:07:50 2024
Response via : Initial Calibration

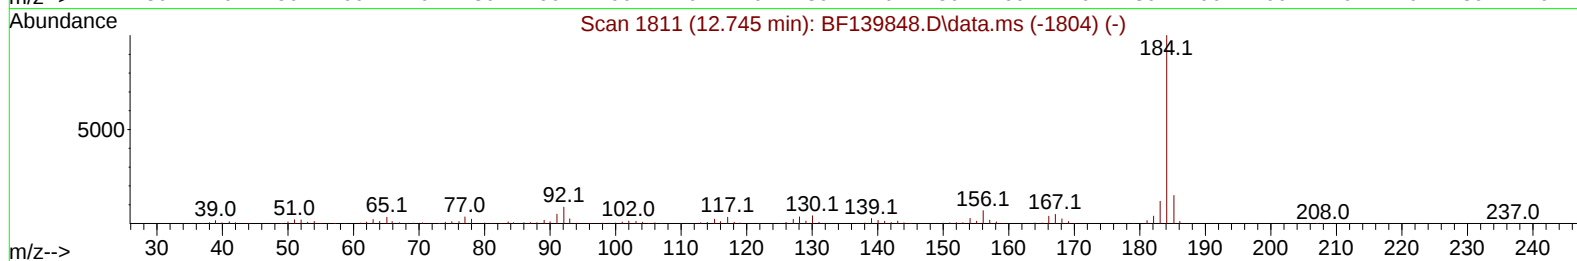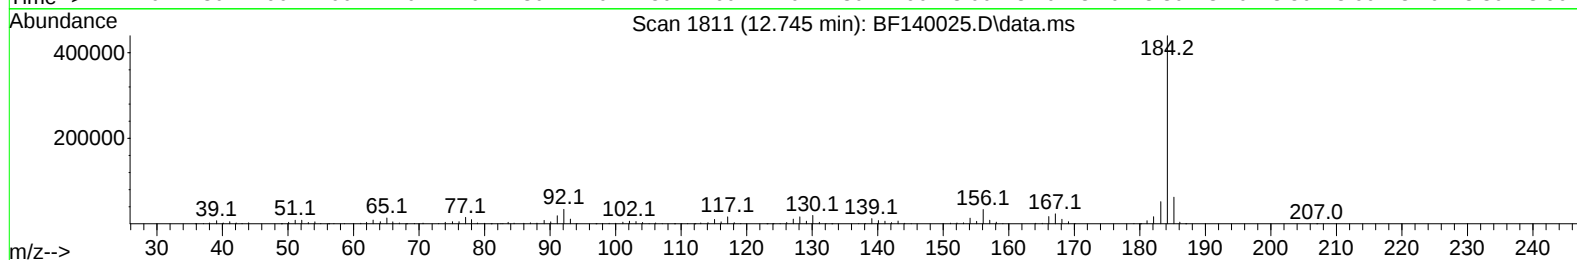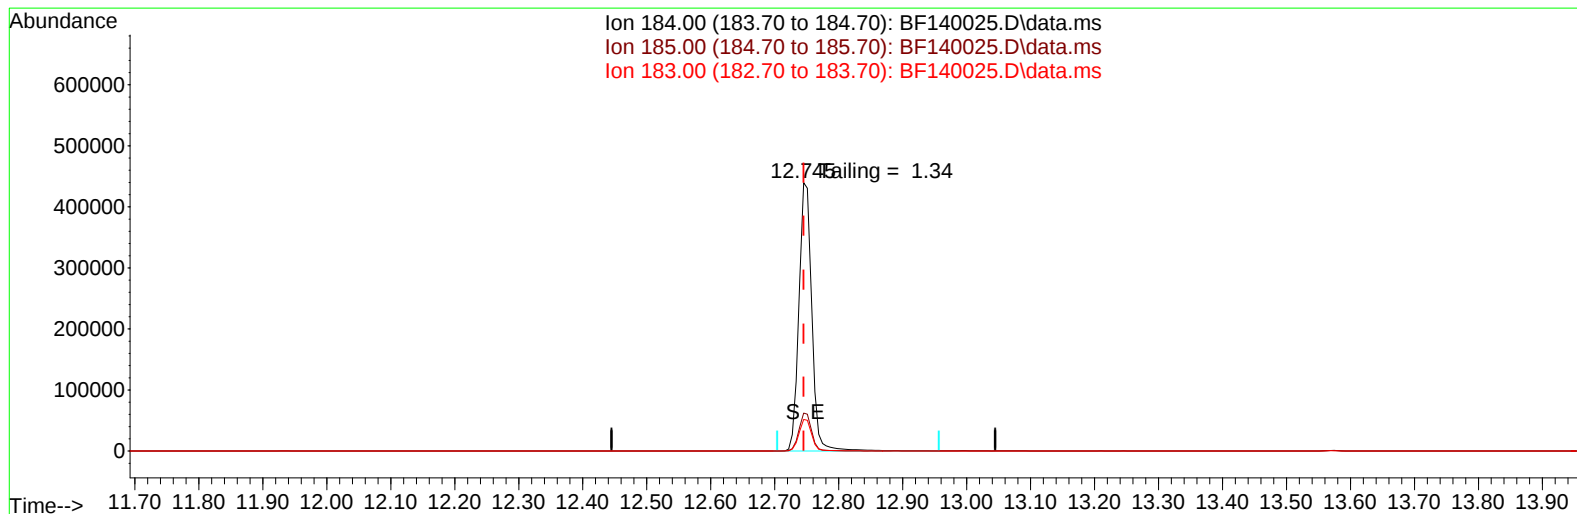

TIC: BF140025.D\data.ms

(77) Benzidine

12.745min (+ 0.000) 95286.91 ng

response 618902

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.00	14.14
183.00	11.80	11.79
0.00	0.00	0.00