
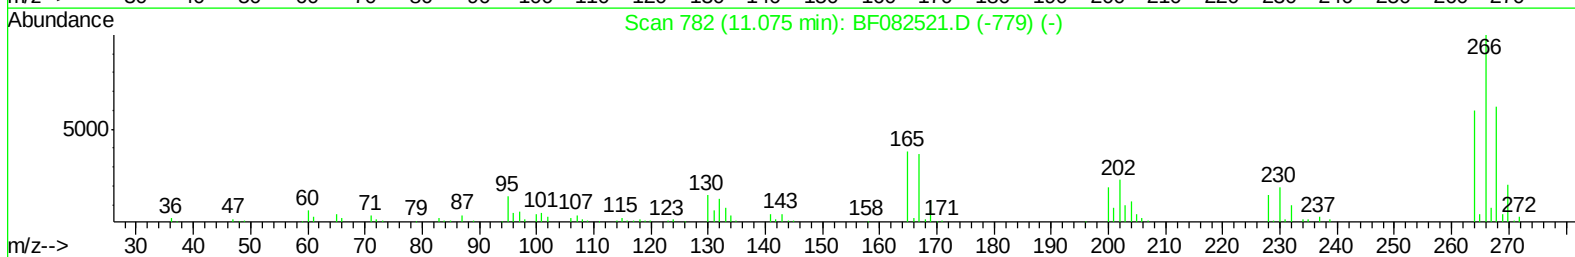
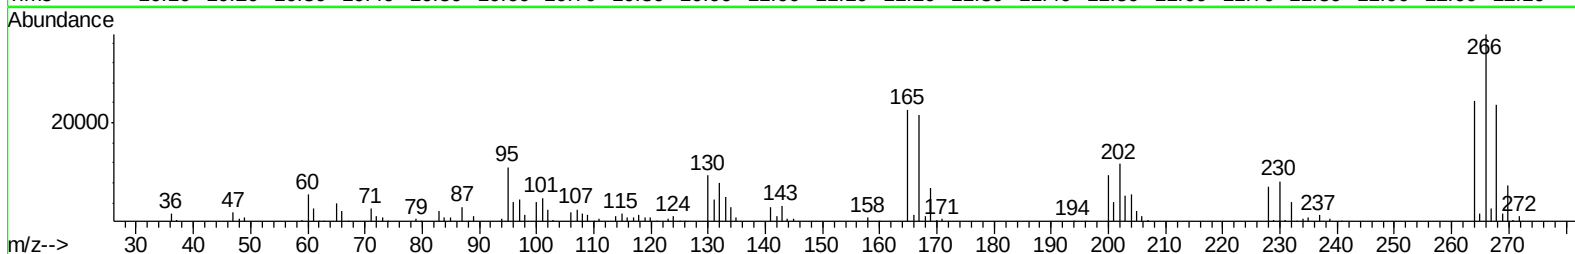


Data Path : Z:\HPCHEM1\BNA F\Data\BF102615\
Data File : BF082517.D
Acq On : 26 Oct 2015 17:19
Operator : UM/IZ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 27 09:06:57 2015
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF102615.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Oct 27 02:43:58 2015
Response via : Initial Calibration

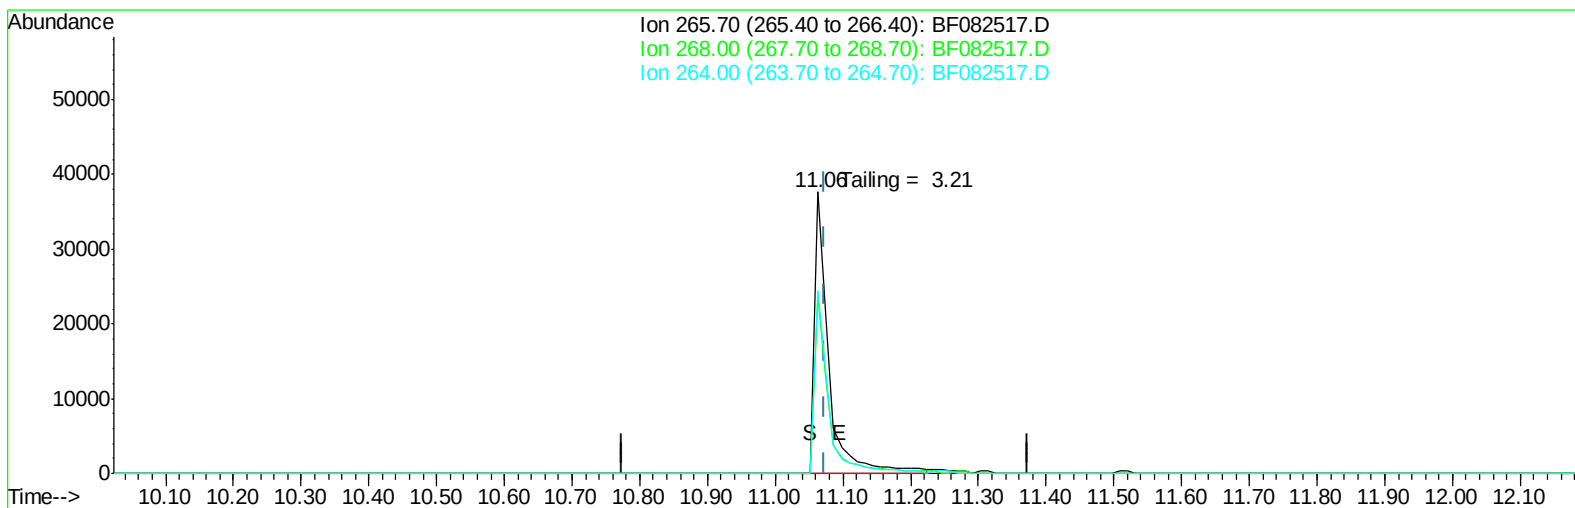

TIC: BF082517.D

(69) Pentachlorophenol (C)




11.064min (-0.010) 0.00ng

response 53696

Ion	Exp%	Act%
265.70	100	100
268.00	61.90	62.79
264.00	60.00	65.00
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA F\Data\BF102615\
Data File : BF082517.D
Acq On : 26 Oct 2015 17:19
Operator : UM/IZ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 27 09:06:57 2015
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF102615.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Oct 27 02:43:58 2015
Response via : Initial Calibration

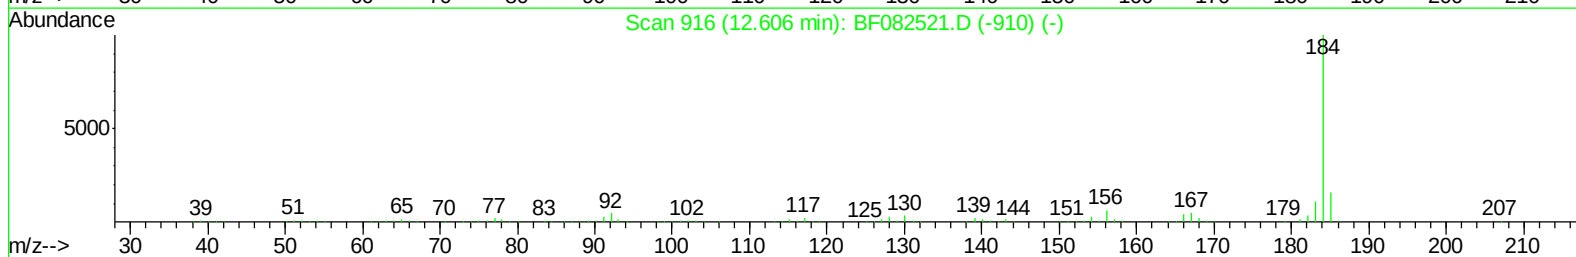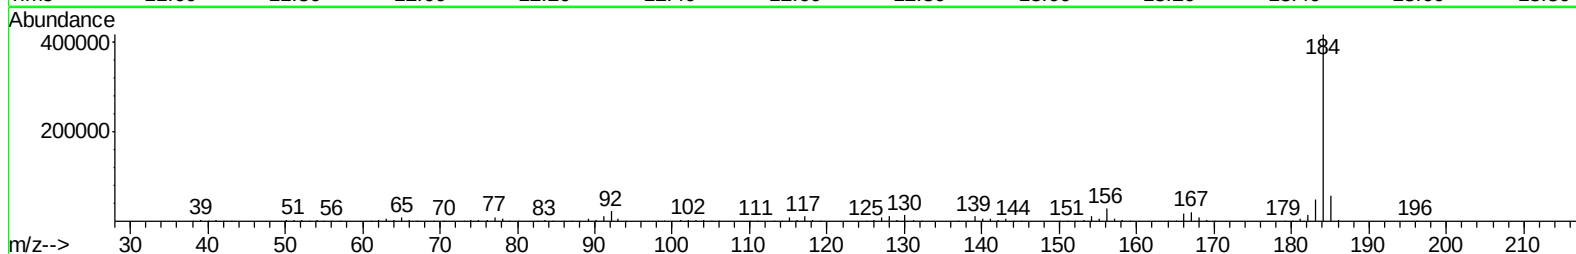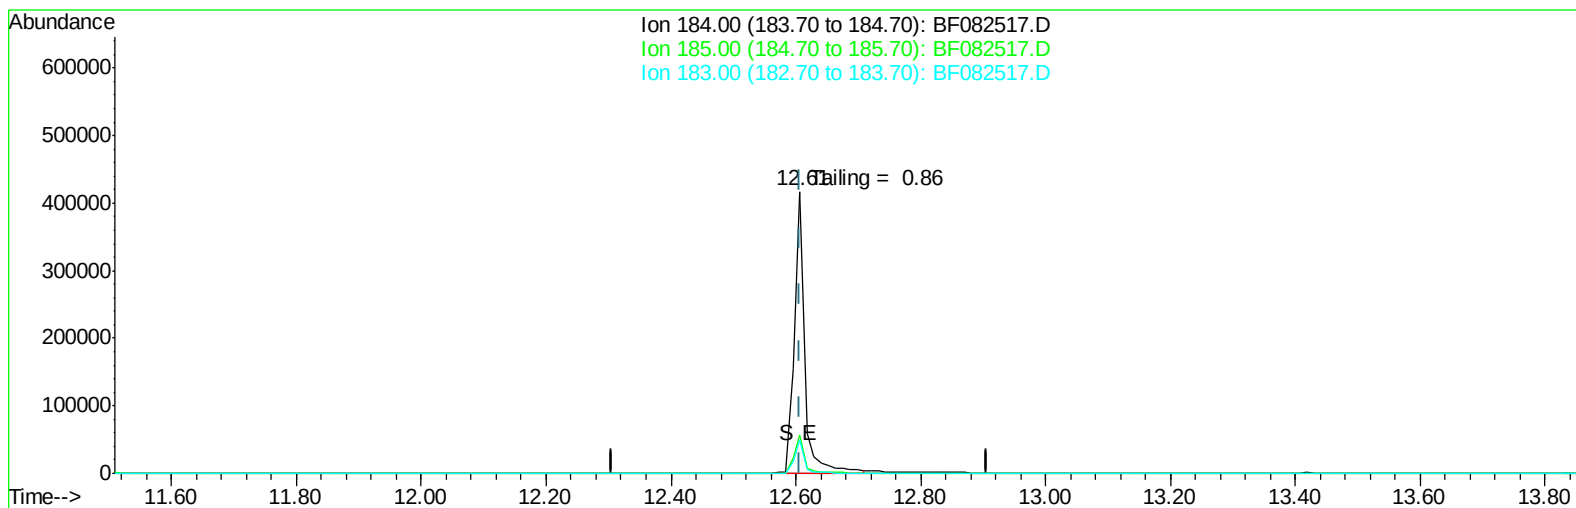

TIC: BF082517.D

(76) Benzidine

12.607min (+0.000) 0.00ng

response 512357

Ion	Exp%	Act%
184.00	100	100
185.00	16.00	13.77
183.00	11.10	11.65
0.00	0.00	0.00