
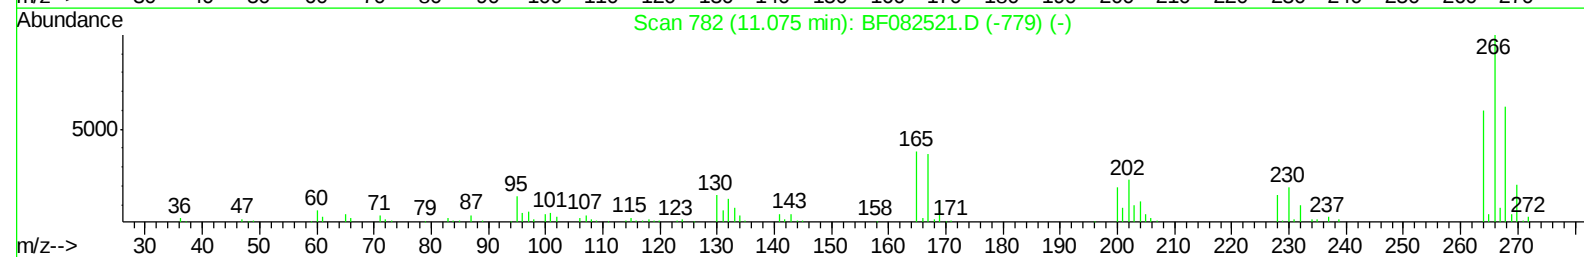
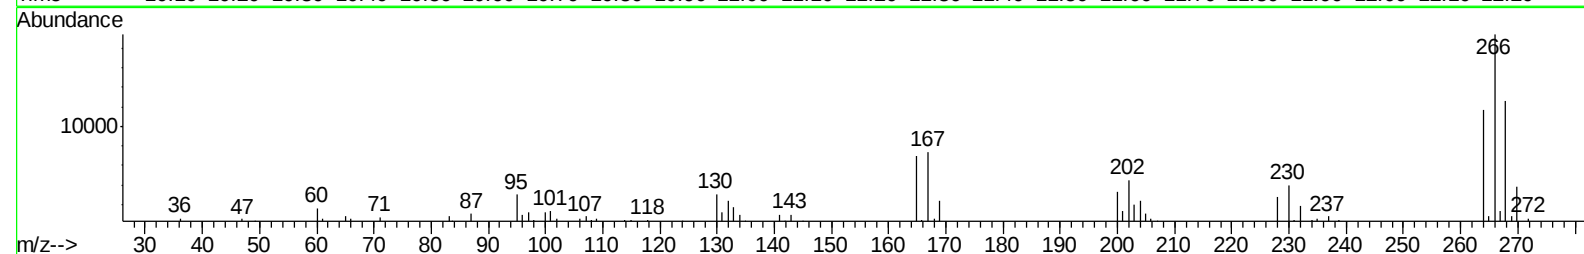


Data Path : Z:\HPCHEM1\BNA F\Data\BF102615\
Data File : BF082526.D
Acq On : 27 Oct 2015 2:10
Operator : UM/IZ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 27 09:08:07 2015
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF102615.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Oct 27 02:43:58 2015
Response via : Initial Calibration

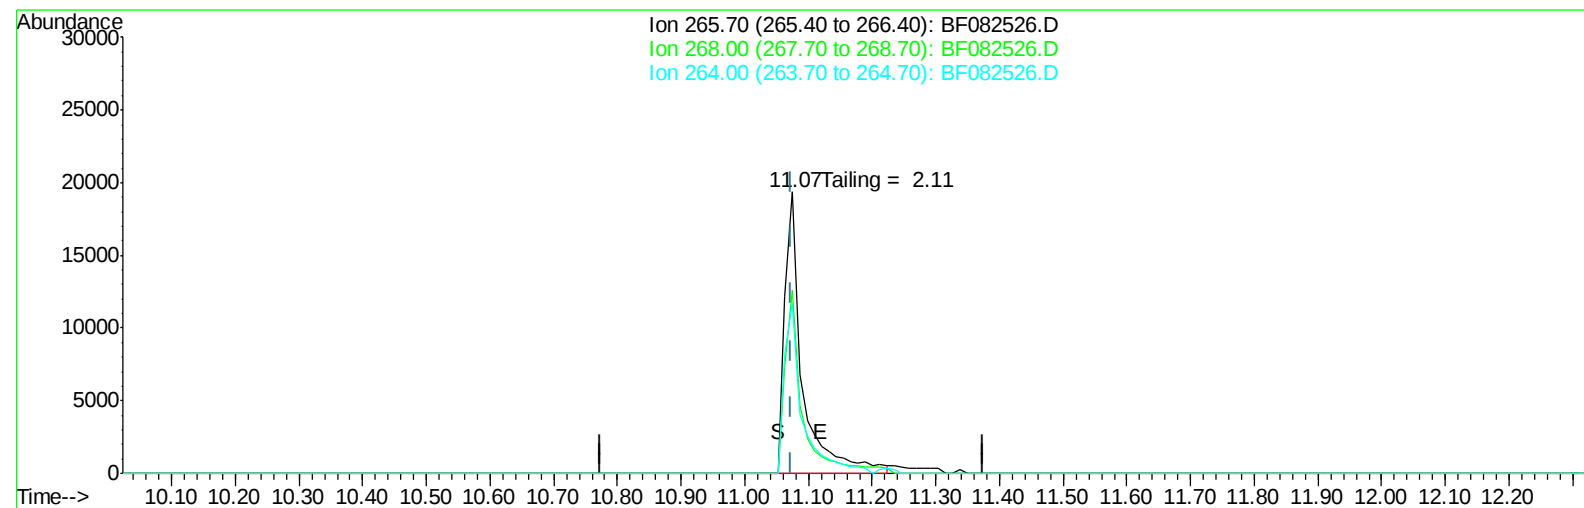

TIC: BF082526.D

(69) Pentachlorophenol (C)




11.075min (+0.001) 42049.50ng

response 38929

Ion	Exp%	Act%
265.70	100	100
268.00	61.90	64.93
264.00	60.00	60.59
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA F\Data\BF102615\
Data File : BF082526.D
Acq On : 27 Oct 2015 2:10
Operator : UM/IZ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 27 09:08:07 2015
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF102615.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Oct 27 02:43:58 2015
Response via : Initial Calibration

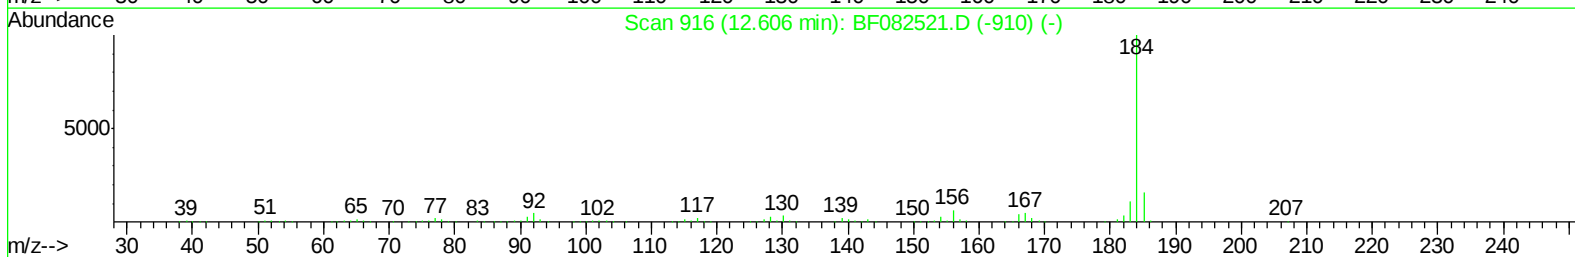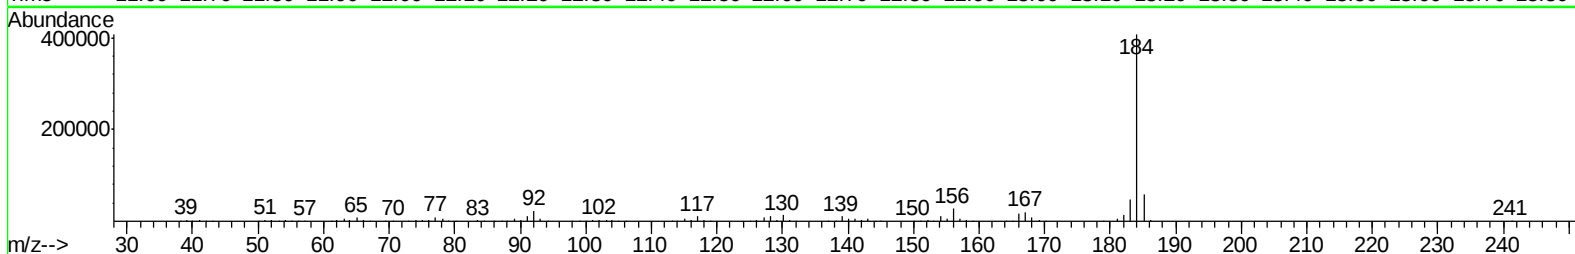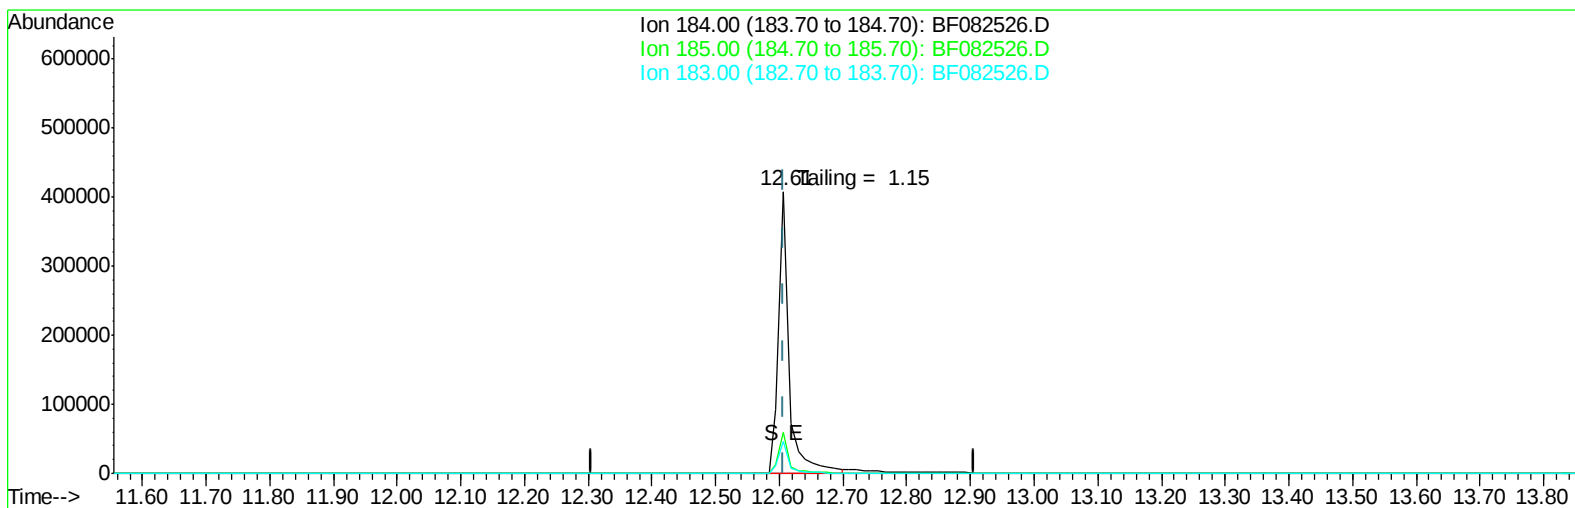

TIC: BF082526.D

(76) Benzidine

12.606min (-0.000) 0.00ng

response 489275

Ion	Exp%	Act%
184.00	100	100
185.00	16.00	14.51
183.00	11.10	11.48
0.00	0.00	0.00