


Data Path : Z:\HPCHEM1\BNA_F\DATA\BF102615\
Data File : BF082517.D
Acq On : 26 Oct 2015 17:19
Operator : UM/IZ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF102615.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Tue Oct 27 02:43:58 2015

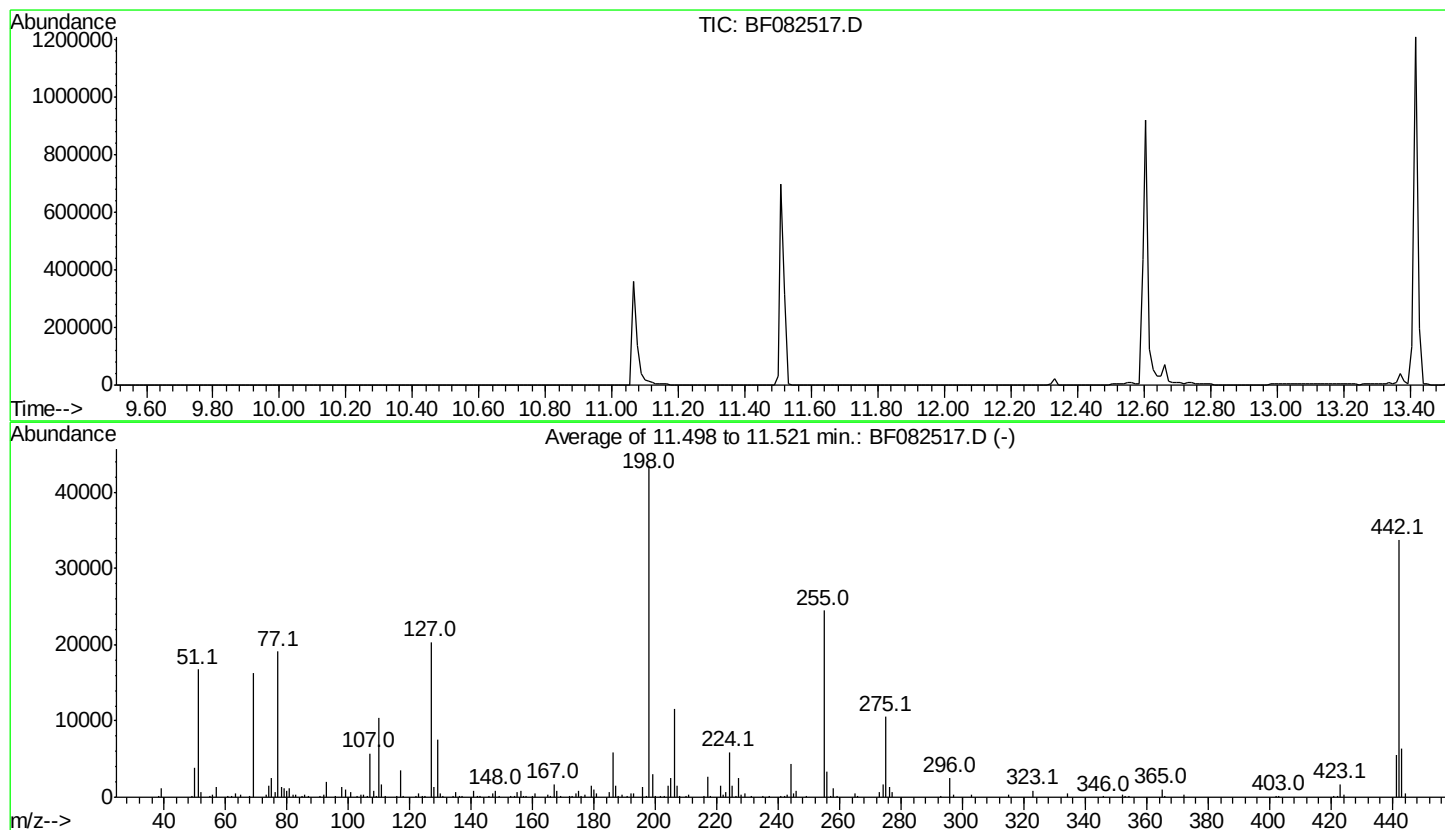

AutoFind: Scans 819, 820, 821; Background Corrected with Scan 816

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	38.5	16768	PASS
68	69	0.00	2	1.1	186	PASS
69	198	0.00	100	37.6	16366	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	46.8	20372	PASS
197	198	0.00	2	0.4	180	PASS
198	198	100	100	100.0	43502	PASS
199	198	5	9	6.9	2988	PASS
275	198	10	60	24.1	10504	PASS
365	198	1	100	2.5	1082	PASS
441	442	0.01	24	16.3	5500	PASS
442	198	50	100	77.6	33763	PASS
443	442	15	24	18.8	6341	PASS