


Data Path : Z:\HPCHEM1\BNA_F\DATA\BF102615\
Data File : BF082526.D
Acq On : 27 Oct 2015 2:10
Operator : UM/IZ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF102615.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Tue Oct 27 02:43:58 2015

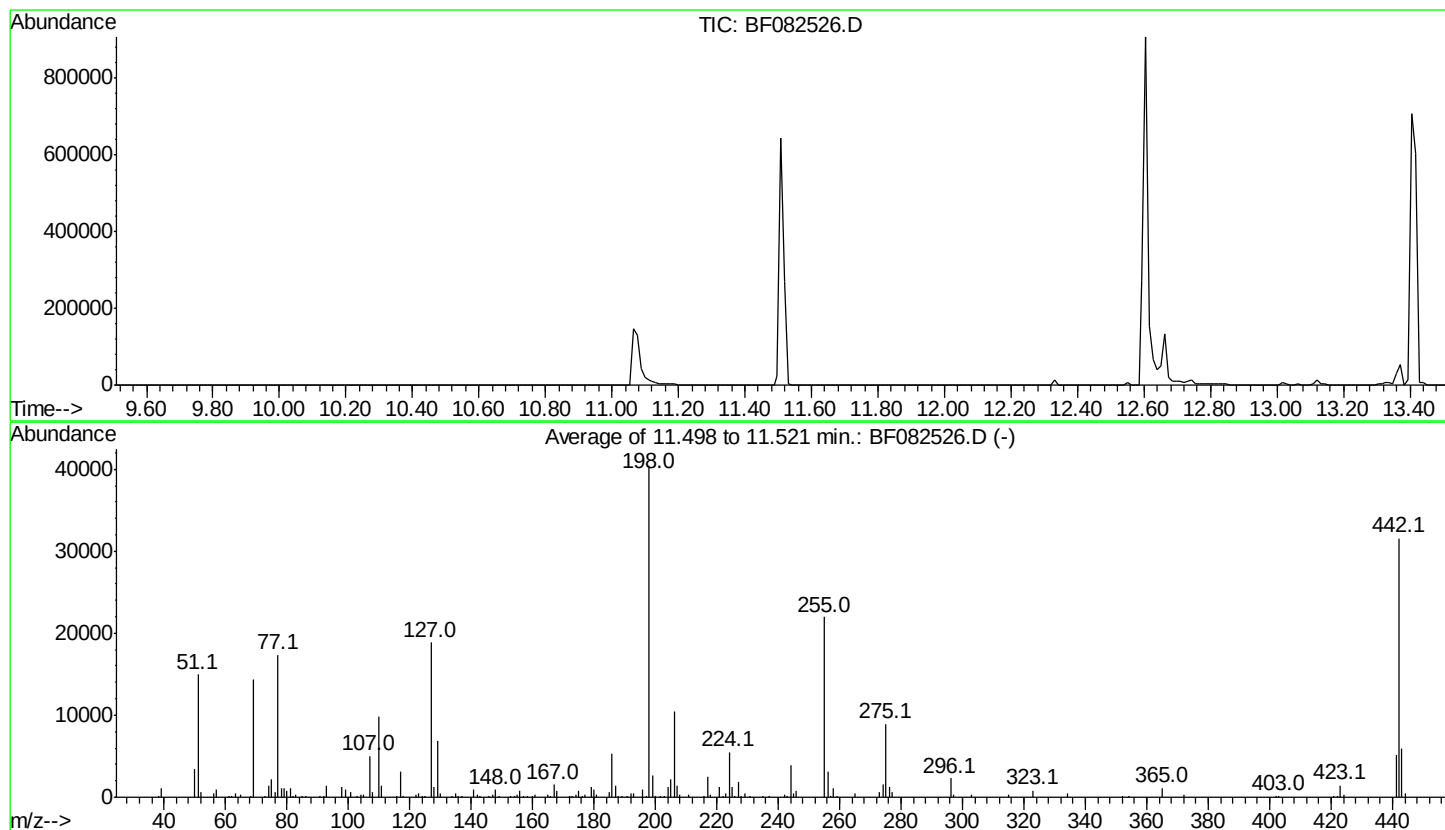

AutoFind: Scans 819, 820, 821; Background Corrected with Scan 816

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	36.9	14926	PASS
68	69	0.00	2	0.9	130	PASS
69	198	0.00	100	35.5	14346	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	46.7	18860	PASS
197	198	0.00	2	0.4	150	PASS
198	198	100	100	100.0	40423	PASS
199	198	5	9	6.5	2640	PASS
275	198	10	60	22.1	8935	PASS
365	198	1	100	2.7	1102	PASS
441	442	0.01	24	16.1	5088	PASS
442	198	50	100	78.1	31562	PASS
443	442	15	24	18.8	5939	PASS