
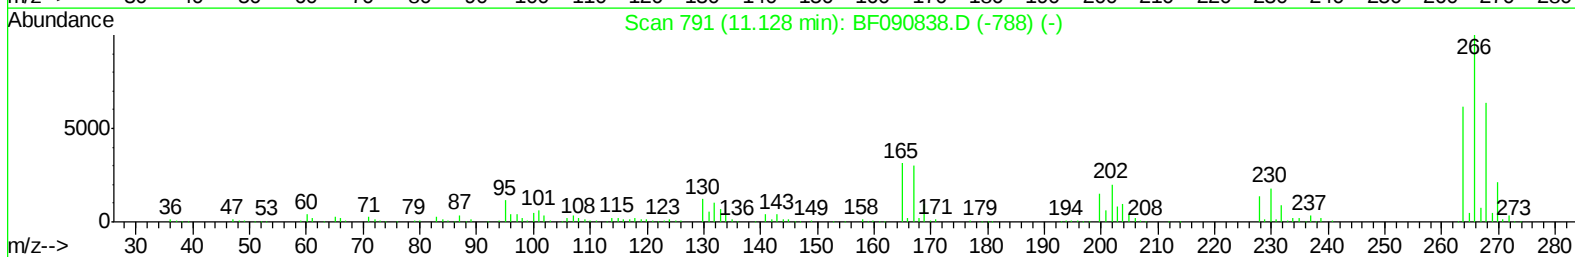
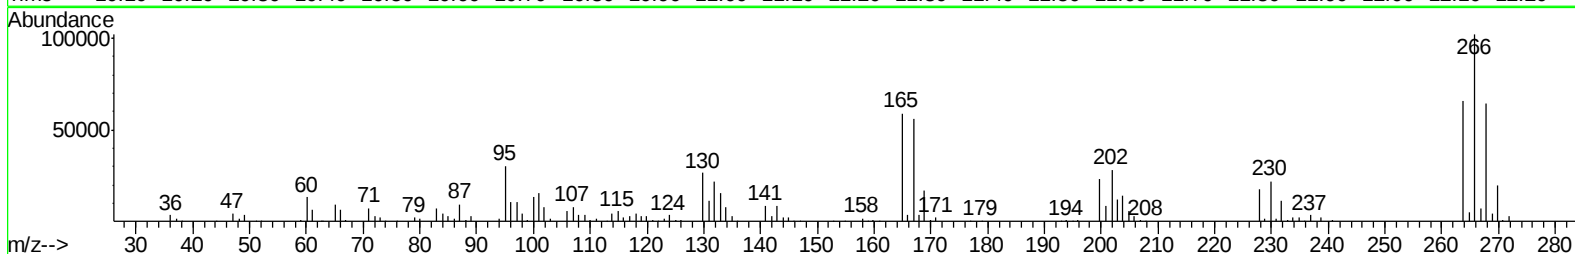


Data Path : Z:\HPCHEM1\BNA_F\DATA\BF102616\
Data File : BF090833.D
Acq On : 26 Oct 2016 10:45
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 27 08:12:06 2016
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF102616.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Oct 26 16:35:31 2016
Response via : Initial Calibration

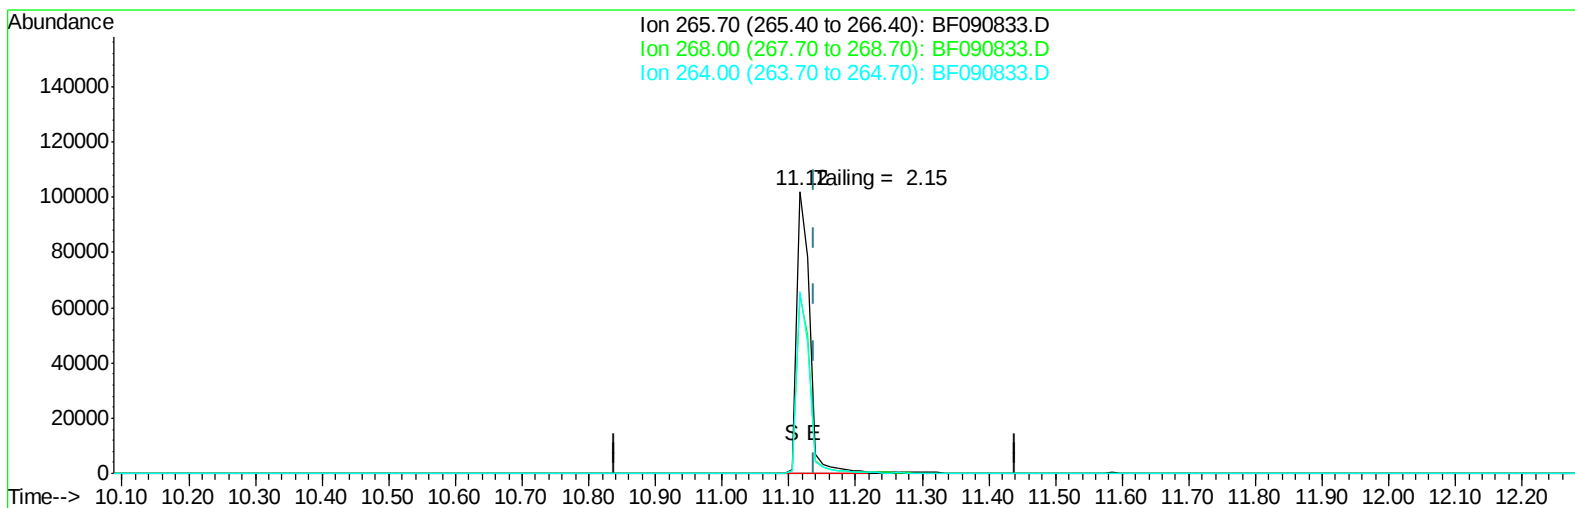

TIC: BF090833.D

(69) Pentachlorophenol (C)




11.116min (-0.023) 0.00ng

response 138908

Ion	Exp%	Act%
265.70	100	100
268.00	62.20	63.27
264.00	62.70	64.45
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF102616\
Data File : BF090833.D
Acq On : 26 Oct 2016 10:45
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 27 08:12:06 2016
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF102616.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Oct 26 16:35:31 2016
Response via : Initial Calibration

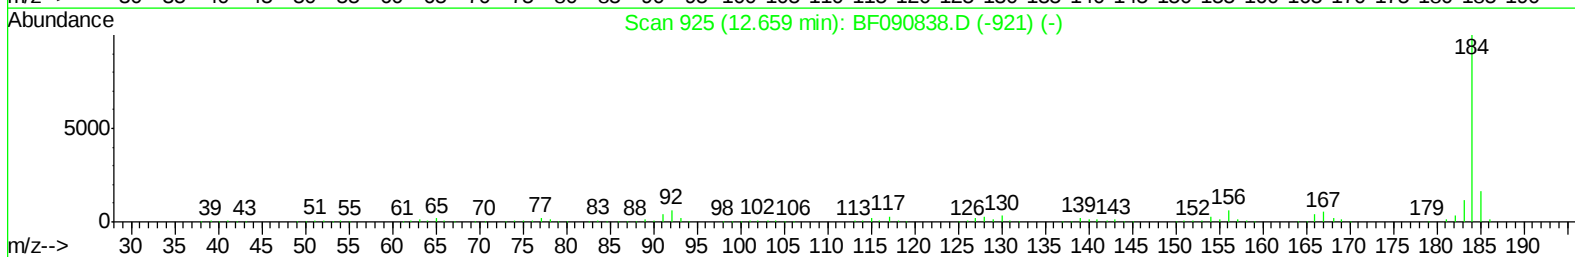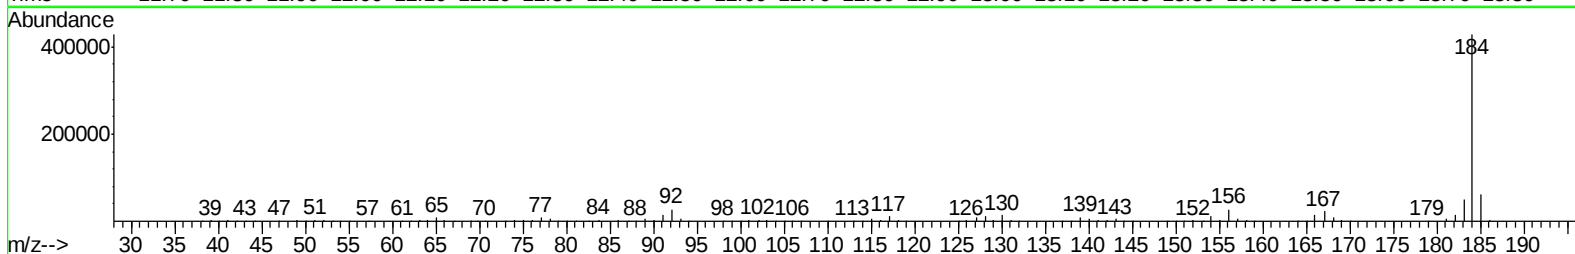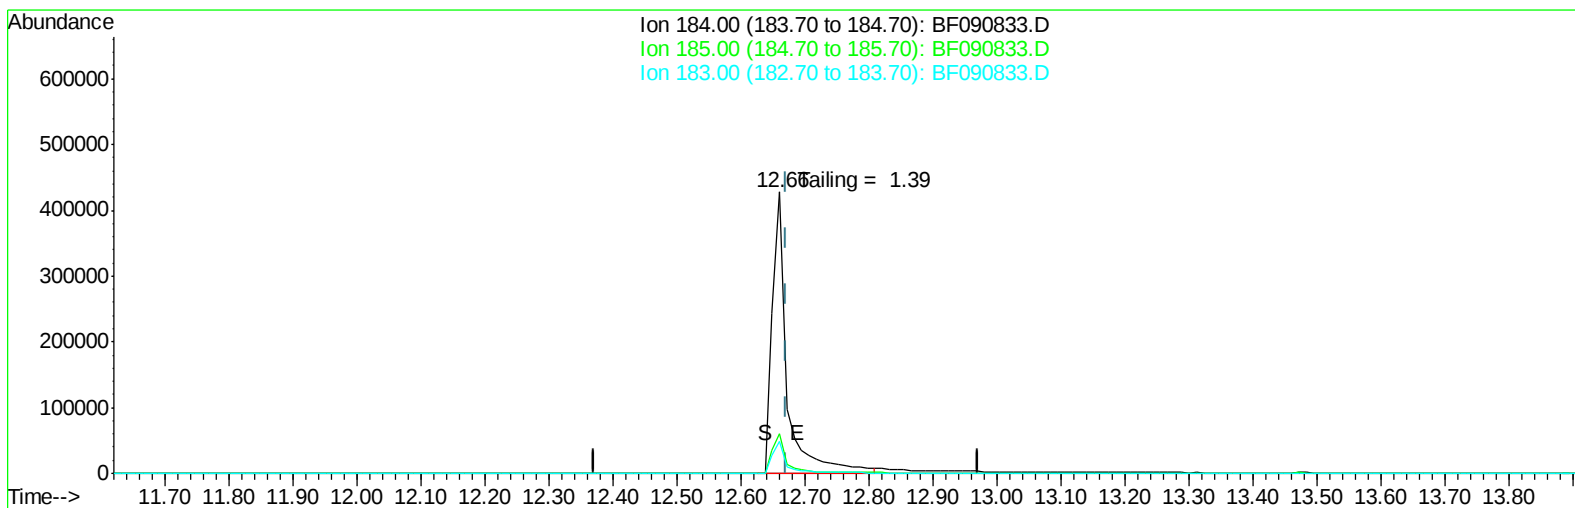

TIC: BF090833.D

(76) Benzidine

12.659min (-0.012) 84778.68ng

response 716387

Ion	Exp%	Act%
184.00	100	100
185.00	14.70	14.30
183.00	9.50	11.53#
0.00	0.00	0.00