
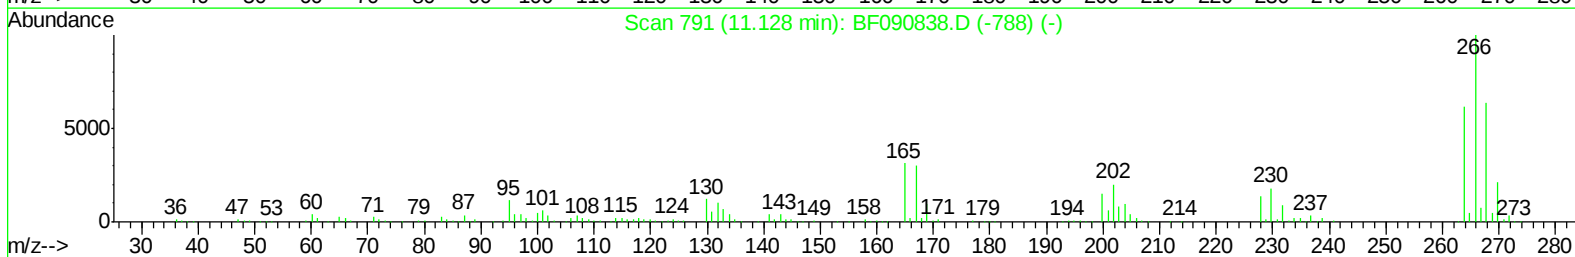
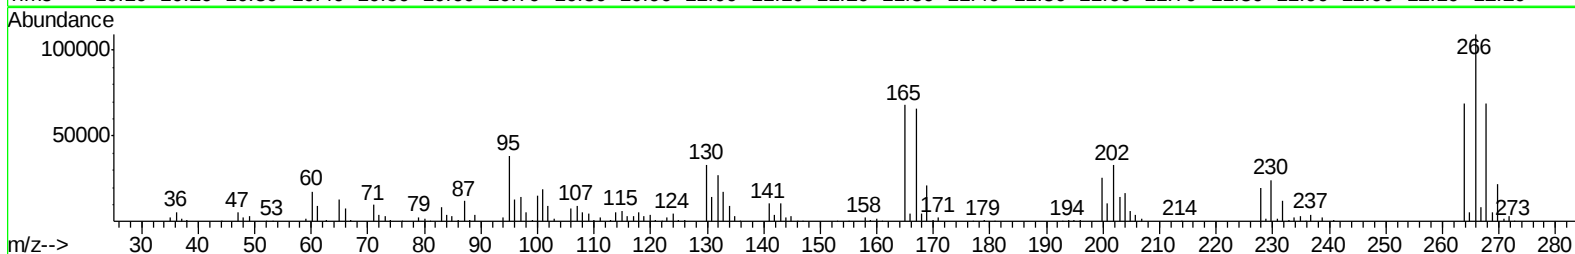


Data Path : Z:\HPCHEM1\BNA_F\DATA\BF102616\
Data File : BF090843.D
Acq On : 26 Oct 2016 15:46
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 27 08:13:11 2016
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF102616.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Oct 26 16:35:31 2016
Response via : Initial Calibration

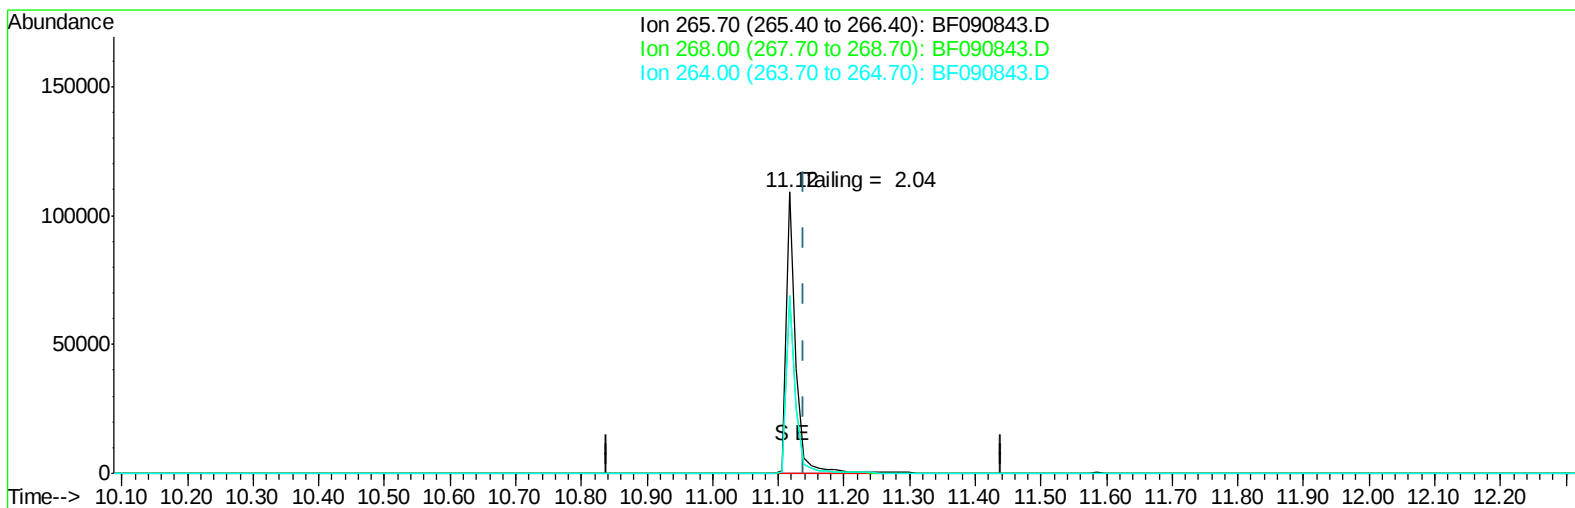

TIC: BF090843.D

(69) Pentachlorophenol (C)




11.116min (-0.023) 0.00ng

response 116473

Ion	Exp%	Act%
265.70	100	100
268.00	62.20	62.81
264.00	62.70	63.41
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF102616\
Data File : BF090843.D
Acq On : 26 Oct 2016 15:46
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 27 08:13:11 2016
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF102616.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Oct 26 16:35:31 2016
Response via : Initial Calibration

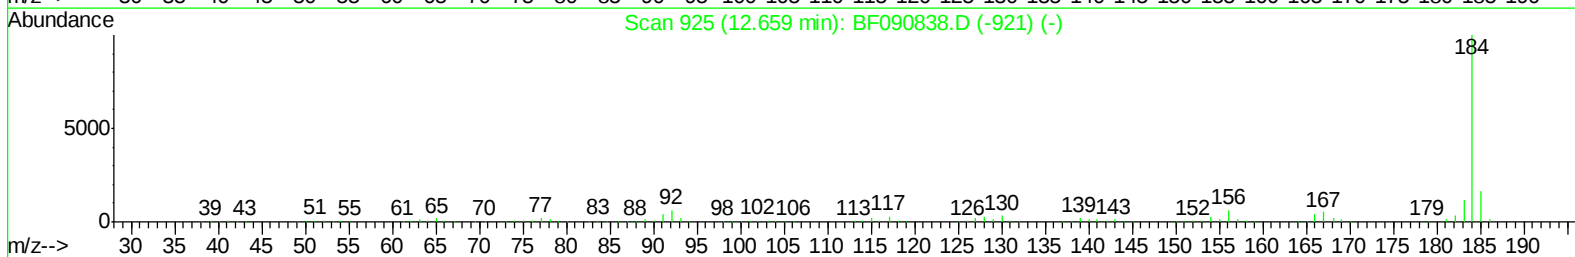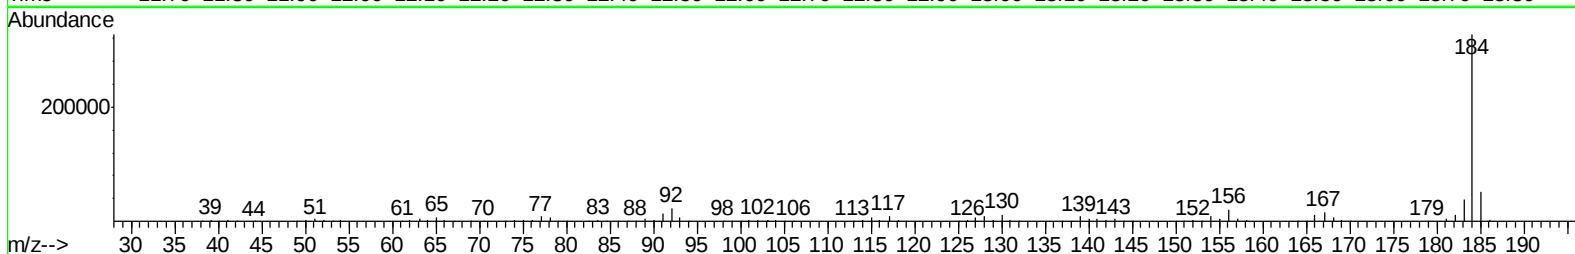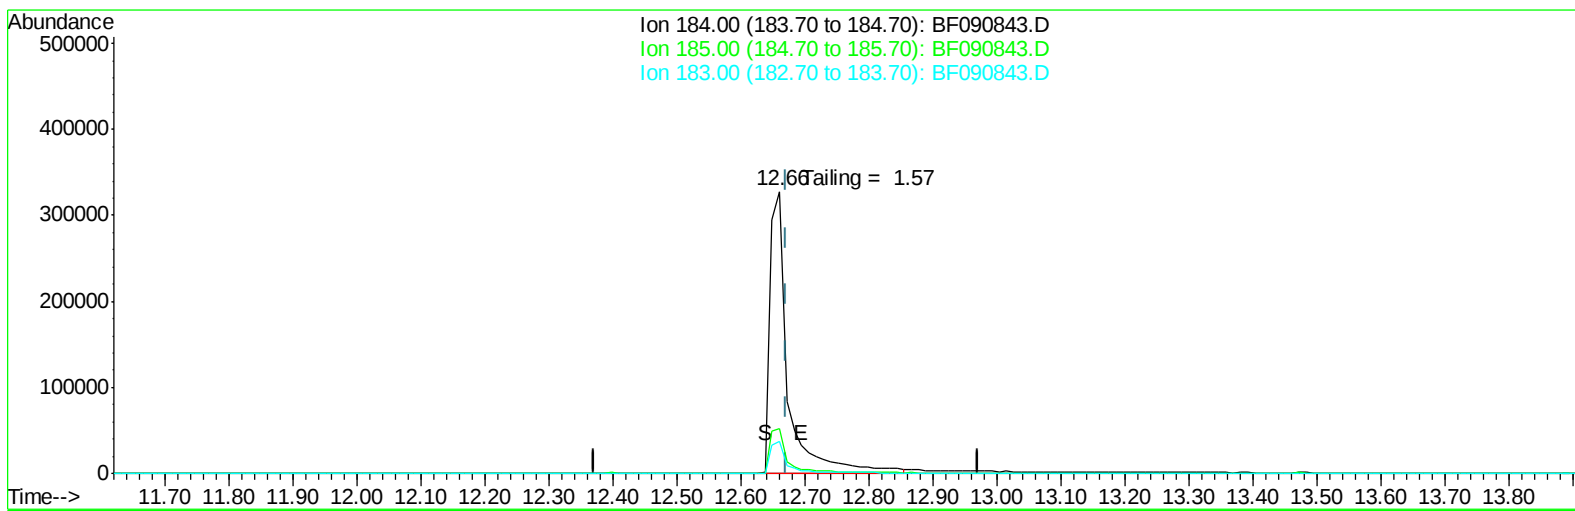

TIC: BF090843.D

(76) Benzidine

12.659min (-0.011) 0.00ng

response 656373

Ion	Exp%	Act%
184.00	100	100
185.00	14.70	15.81
183.00	9.50	11.50#
0.00	0.00	0.00