

Data Path : Z:\HPCHEM1\BNA F\DATA\BF102616\
 Data File : BF090850.D
 Acq On : 26 Oct 2016 19:55
 Operator : UM/SJ
 Sample : PB94315TB
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PB94315TB

Quant Time: Oct 27 02:19:35 2016
 Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF102616.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Oct 26 16:35:31 2016
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	6.78	152	166989	20.00	ng	-0.01
21) Naphthalene-d8	8.08	136	684226	20.00	ng	-0.01
38) Acenaphthene-d10	9.82	164	364410	20.00	ng	-0.02
63) Phenanthrene-d10	11.31	188	664363	20.00	ng	-0.01
75) Chrysene-d12	13.95	240	593651	20.00	ng	-0.01
86) Perylene-d12	15.37	264	448841	20.00	ng	-0.01
System Monitoring Compounds						
5) 2-Fluorophenol	5.39	112	1178793	123.42	ng	0.00
7) Phenol-d6	6.43	99	1557012	120.84	ng	-0.01
23) Nitrobenzene-d5	7.36	82	892024	85.35	ng	-0.01
41) 2,4,6-Tribromophenol	10.62	330	452629	120.86	ng	-0.01
44) 2-Fluorobiphenyl	9.15	172	1673285	80.63	ng	-0.02
78) Terphenyl-d14	12.90	244	2009693	85.29	ng	-0.02


Target Compounds Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA F\DATA\BF102616\
Data File : BF090850.D
Acq On : 26 Oct 2016 19:55
Operator : UM/SJ
Sample : PB94315TB
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB94315TB

Quant Time: Oct 27 02:19:35 2016
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF102616.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Oct 26 16:35:31 2016
Response via : Initial Calibration

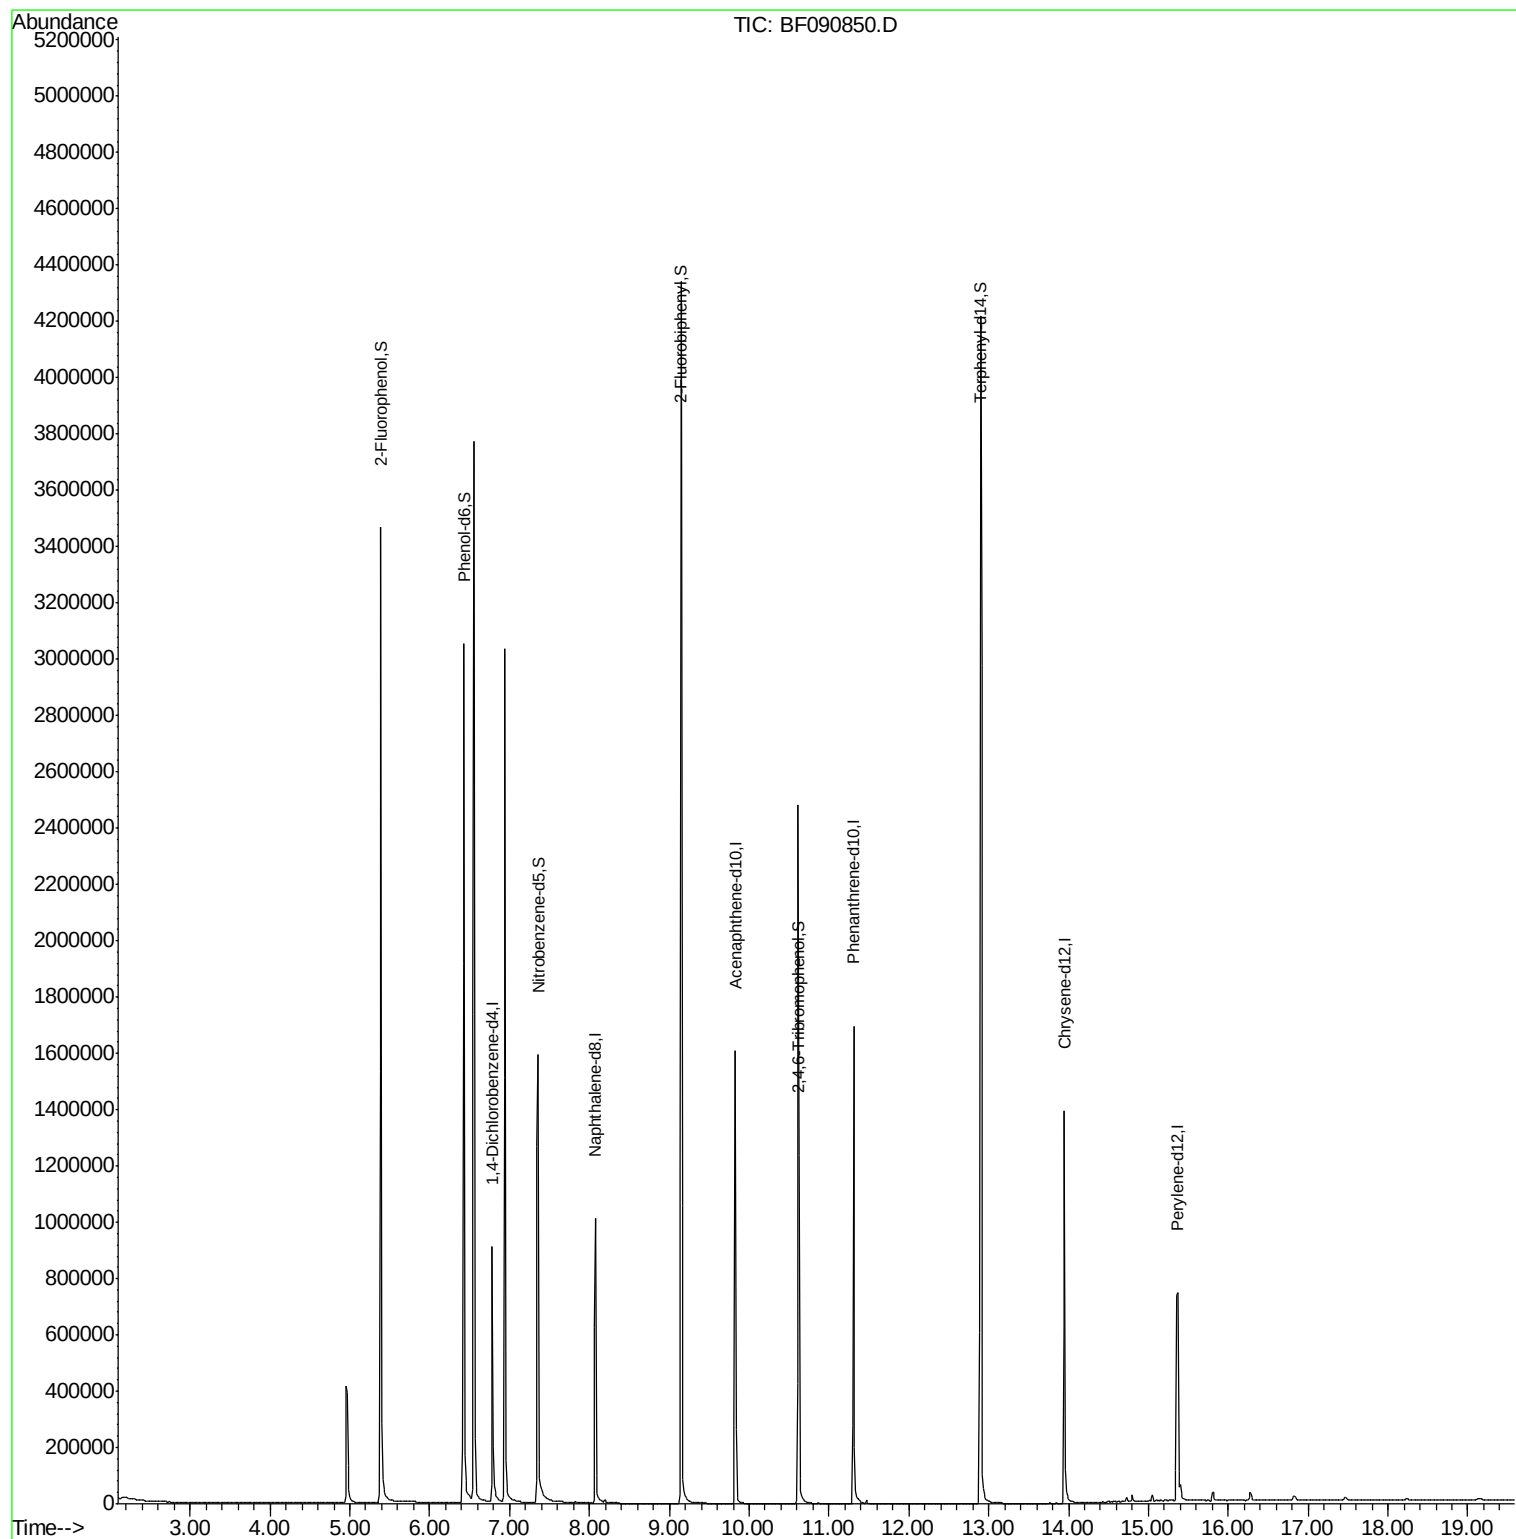

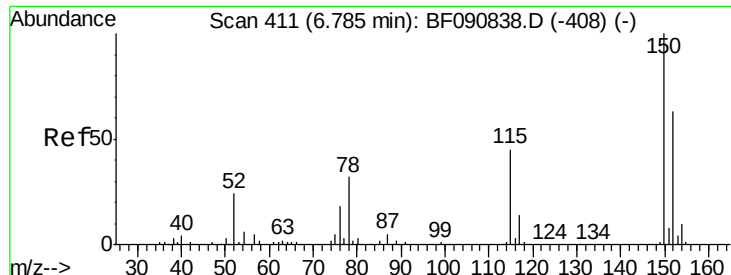


#1




1,4-Dichlorobenzene-d4
Concen: 20.00 ng
RT: 6.78 min Scan# 411
Delta R.T. -0.01 min
Lab File: BF090850.D
Acq: 26 Oct 2016 19:55

Instrument :
BNA_F
ClientSampleId :
PB94315TB

Tot Ion:152 Resp: 166989
Ion Ratio Lower Upper
152 100
150 156.2 124.7 187.1
115 60.5 39.0 58.4#

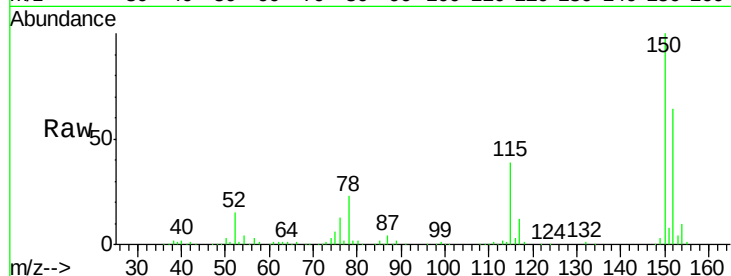


Abundance Ion 152.00 (151.70 to 152.70): E
Ion 150.00 (149.70 to 150.70): E
Ion 115.00 (114.70 to 115.70): E

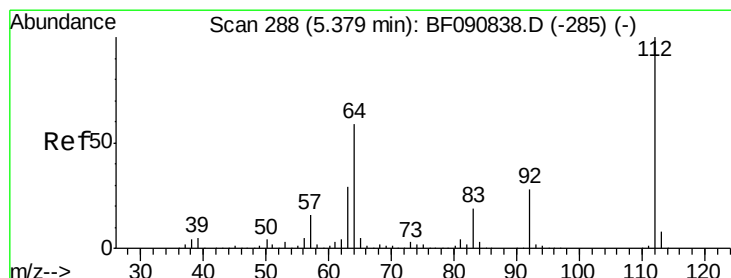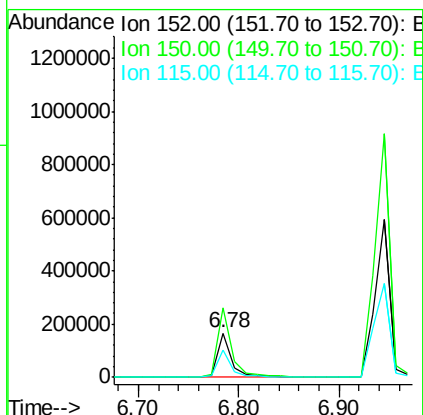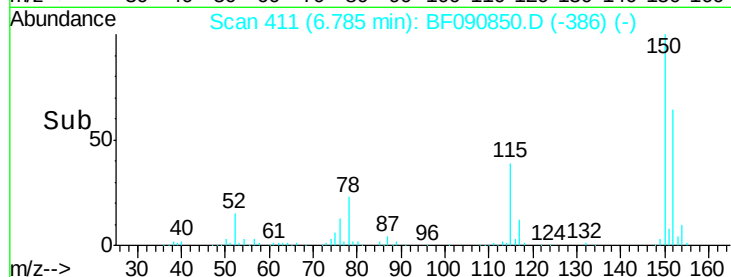



#5


2-Fluorophenol
Concen: 123.42 ng
RT: 5.39 min Scan# 289
Delta R.T. 0.00 min
Lab File: BF090850.D
Acq: 26 Oct 2016 19:55

Tgt Ion:112 Resp: 1178793
Ion Ratio Lower Upper
112 100
64 55.9 39.7 59.5
63 28.1 17.4 26.0#

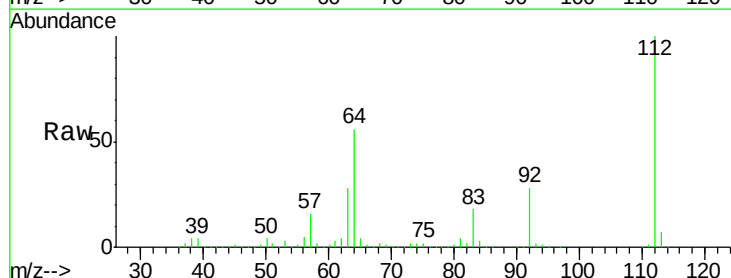

Abundance Ion 112.00 (111.70 to 112.70): E
Ion 64.00 (63.70 to 64.70): BF0
Ion 63.00 (62.70 to 63.70): BF0

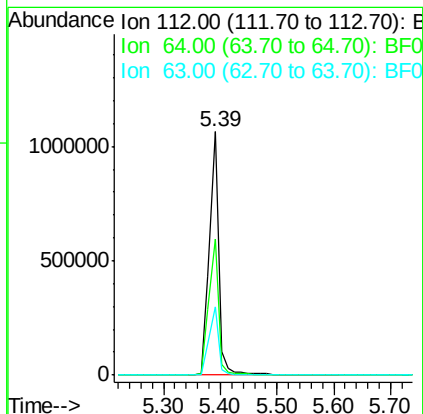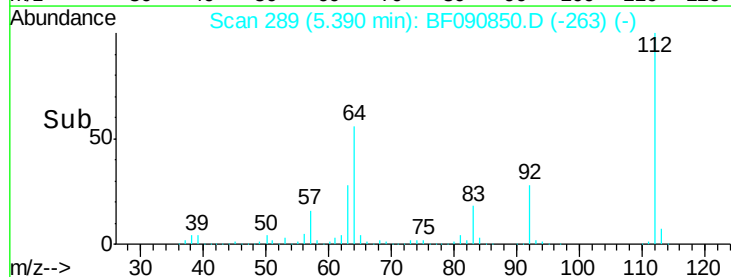

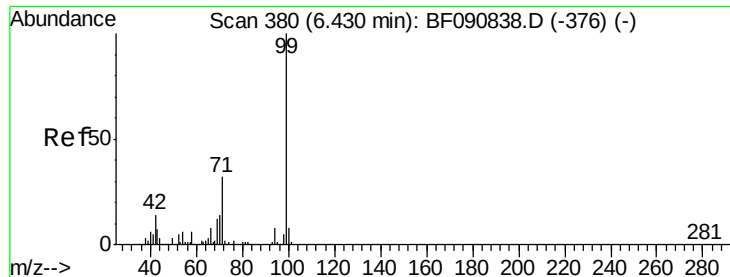

#7

Phenol-d6

Concen: 120.84 ng

RT: 6.43 min Scan# 380

Delta R.T. -0.01 min

Lab File: BF090850.D

Acq: 26 Oct 2016 19:55

Instrument :

BNA_F

ClientSampleId :

PB94315TB


Tot Ion: 99 Resp: 1557012

Ion Ratio Lower Upper

99 100

42 12.9 13.7 20.5#




71 30.8 14.2 21.2#

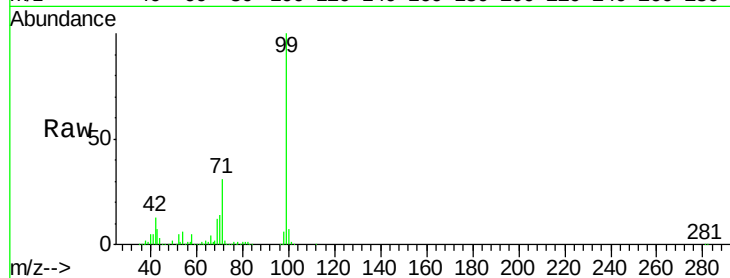

Abundance Ion 99.00 (98.70 to 99.70): BF0

Ion 42.00 (41.70 to 42.70): BF0

Ion 71.00 (70.70 to 71.70): BF0

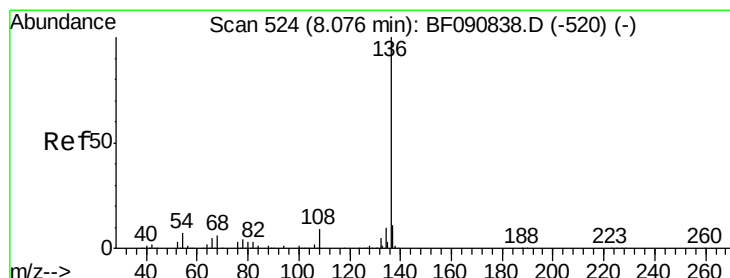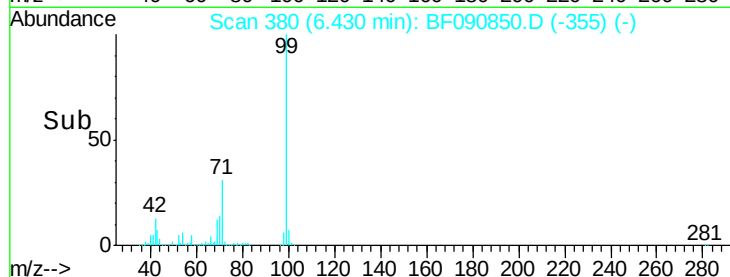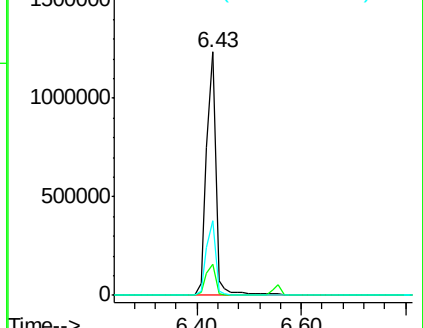

#21

Naphthalene-d8

Concen: 20.00 ng

RT: 8.08 min Scan# 524

Delta R.T. -0.01 min

Lab File: BF090850.D

Acq: 26 Oct 2016 19:55

Tgt Ion: 136 Resp: 684226


Ion Ratio Lower Upper

136 100

137 10.8 9.0 13.6

54 5.2 8.2 12.2#

68 5.1 5.8 8.6#


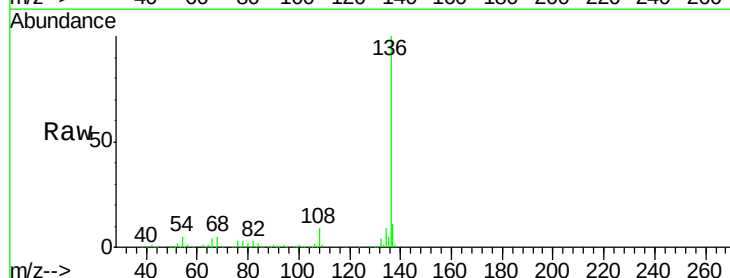



Abundance Ion 136.00 (135.70 to 136.70): E

Ion 137.00 (136.70 to 137.70): E

Ion 54.00 (53.70 to 54.70): BF0

Ion 68.00 (67.70 to 68.70): BF0



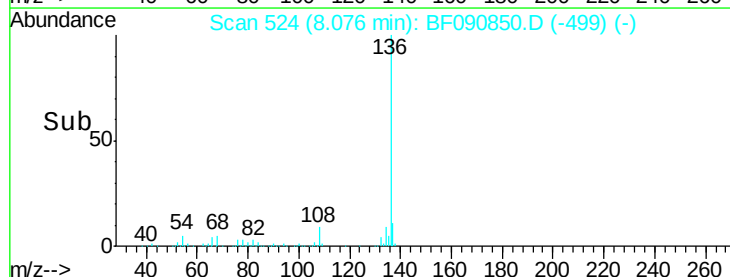
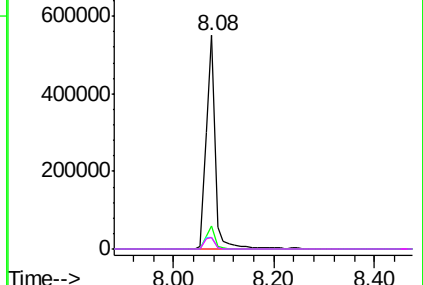


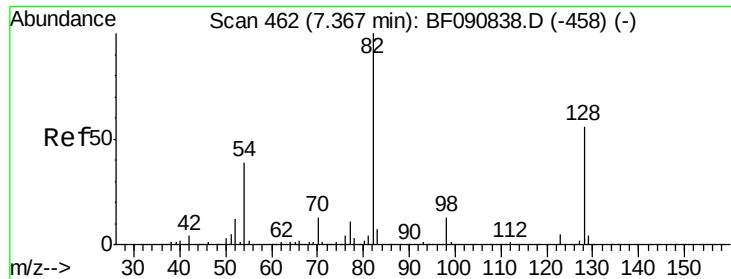

#23
 Nitrobenzene-d5
 Concen: 85.35 ng
 RT: 7.36 min Scan# 461
 Delta R.T. -0.01 min
 Lab File: BF090850.D
 Acq: 26 Oct 2016 19:55




Instrument :
 BNA_F
 ClientSampleId :
 PB94315TB


Tot Ion	82	Resp	892024
Ion Ratio	Lower	Upper	
82	100		
128	56.2	51.0	76.6
54	37.7	47.5	71.3#

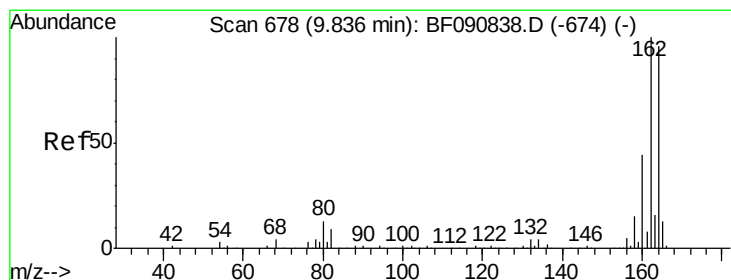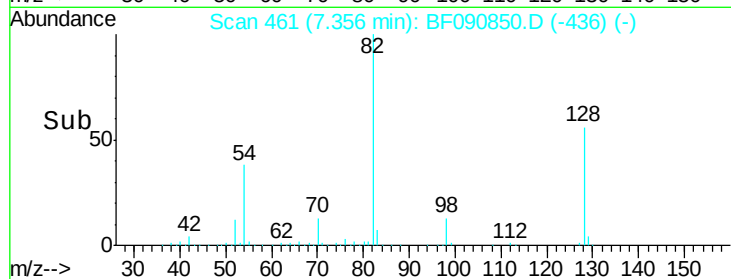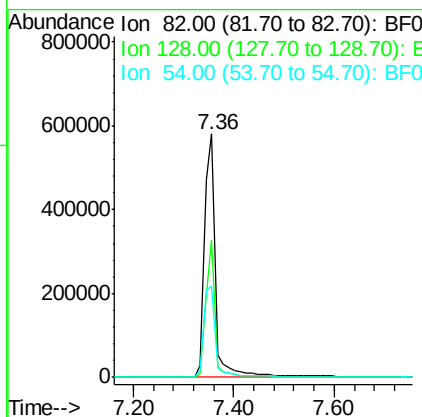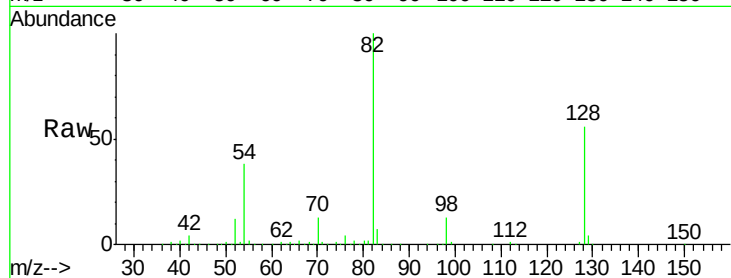

#38
 Acenaphthene-d10
 Concen: 20.00 ng
 RT: 9.82 min Scan# 677
 Delta R.T. -0.02 min
 Lab File: BF090850.D
 Acq: 26 Oct 2016 19:55

Tgt Ion	164	Resp	364410
Ion Ratio	Lower	Upper	
164	100		
162	104.6	75.2	112.8
160	47.0	31.5	47.3

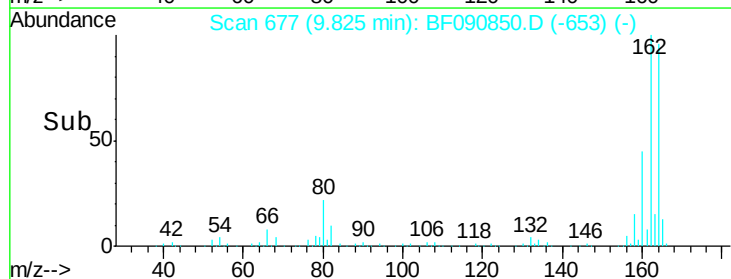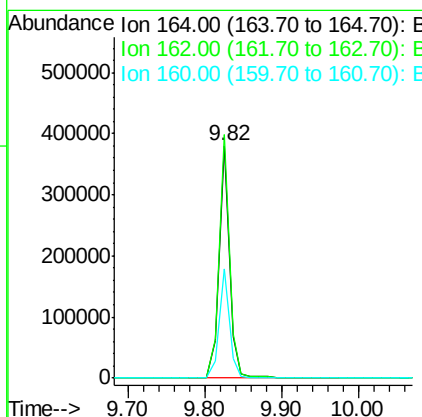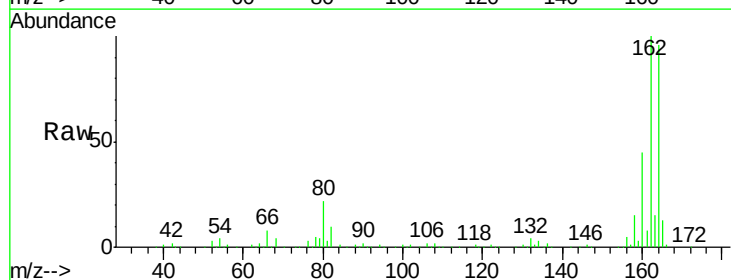


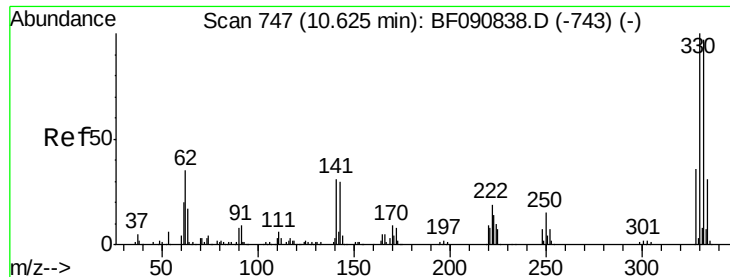




#41
 2,4,6-Tribromophenol
 Concen: 120.86 ng
 RT: 10.62 min Scan# 747
 Delta R.T. -0.01 min
 Lab File: BF090850.D
 Acq: 26 Oct 2016 19:55

Instrument :
 BNA_F
 ClientSampleId :
 PB94315TB

Tot Ion:330 Resp: 452629
 Ion Ratio Lower Upper
 330 100
 332 96.3 76.6 114.8
 141 28.3 29.7 44.5#

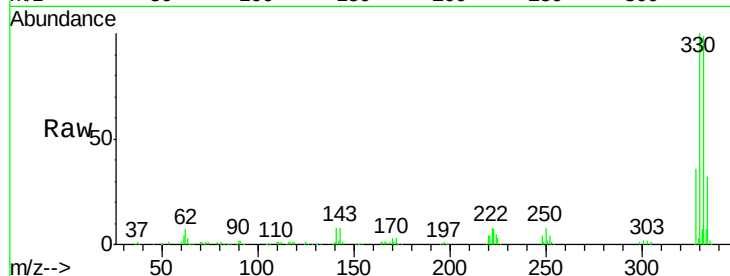


Abundance Ion 329.80 (329.50 to 330.50): E
 Ion 331.80 (331.50 to 332.50): E
 Ion 141.00 (140.70 to 141.70): E

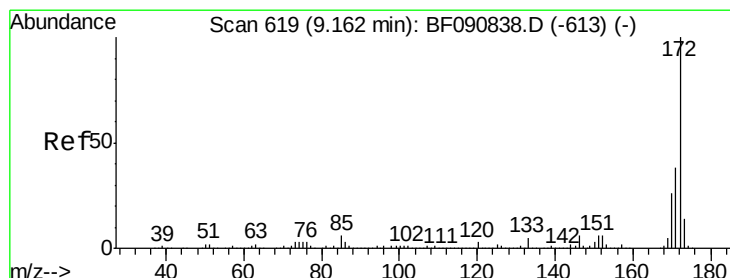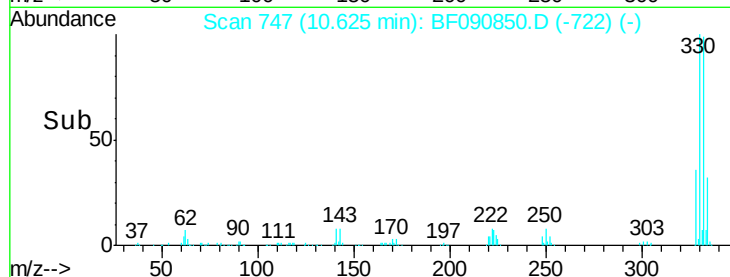
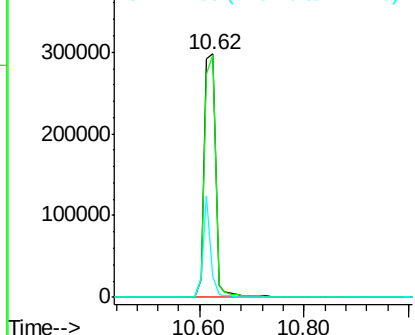



#44
 2-Fluorobiphenyl
 Concen: 80.63 ng
 RT: 9.15 min Scan# 618
 Delta R.T. -0.02 min
 Lab File: BF090850.D
 Acq: 26 Oct 2016 19:55

Tgt Ion:172 Resp: 1673285
 Ion Ratio Lower Upper
 172 100
 171 36.7 26.1 39.1
 170 24.9 17.4 26.2

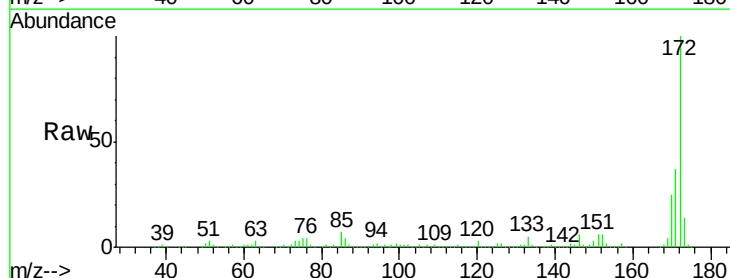

Abundance Ion 172.00 (171.70 to 172.70): E
 Ion 171.00 (170.70 to 171.70): E
 Ion 170.00 (169.70 to 170.70): E

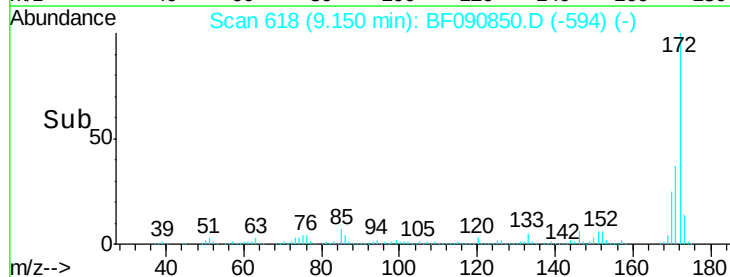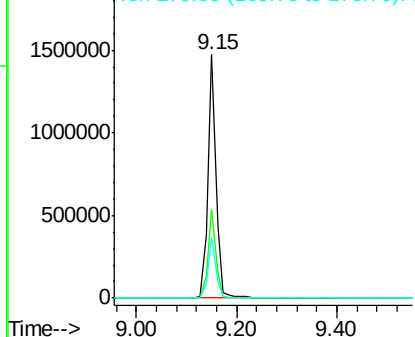


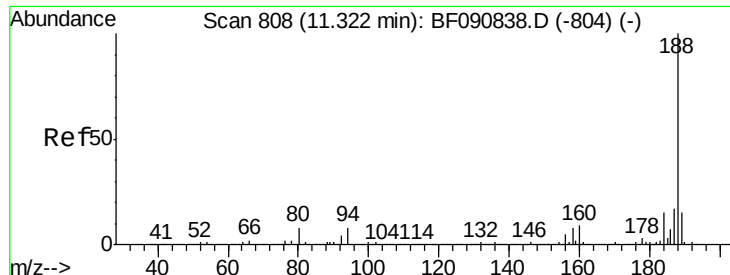




#63
Phenanthrene-d10
Concen: 20.00 ng
RT: 11.31 min Scan# 807
Delta R.T. -0.01 min
Lab File: BF090850.D
Acq: 26 Oct 2016 19:55

Instrument :
BNA_F
ClientSampleId :
PB94315TB

Tot Ion:188 Resp: 664363
Ion Ratio Lower Upper
188 100
94 9.8 11.1 16.7#
80 10.6 11.0 16.4#

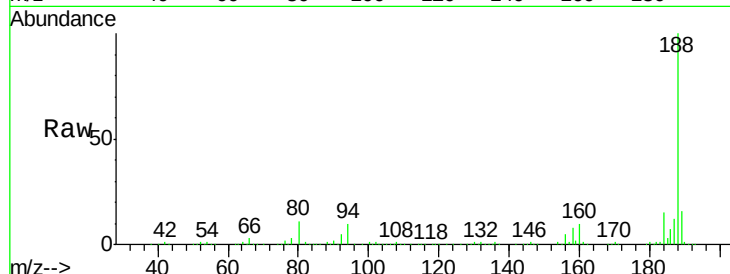


Abundance Ion 188.00 (187.70 to 188.70): E
Ion 94.00 (93.70 to 94.70): BF0
Ion 80.00 (79.70 to 80.70): BF0

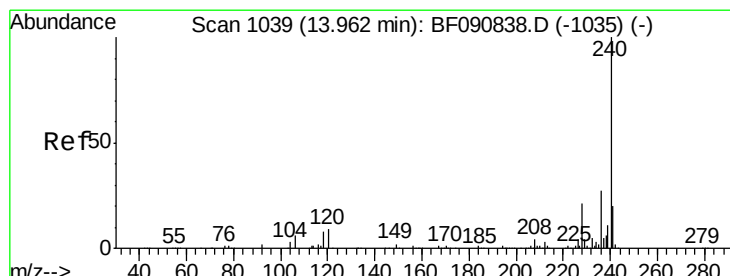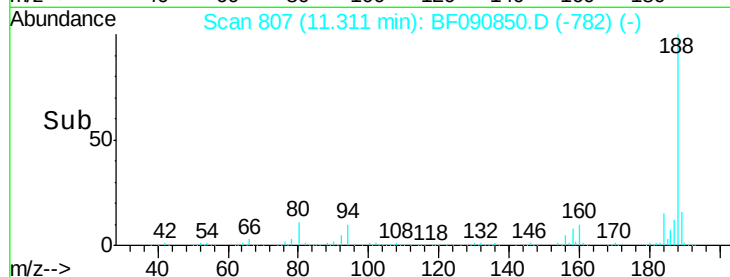
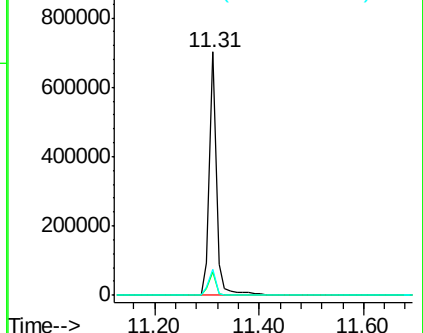



#75
Chrysene-d12
Concen: 20.00 ng
RT: 13.95 min Scan# 1038
Delta R.T. -0.01 min
Lab File: BF090850.D
Acq: 26 Oct 2016 19:55

Tgt Ion:240 Resp: 593651
Ion Ratio Lower Upper
240 100
120 9.2 16.2 24.2#
236 26.6 18.4 27.6

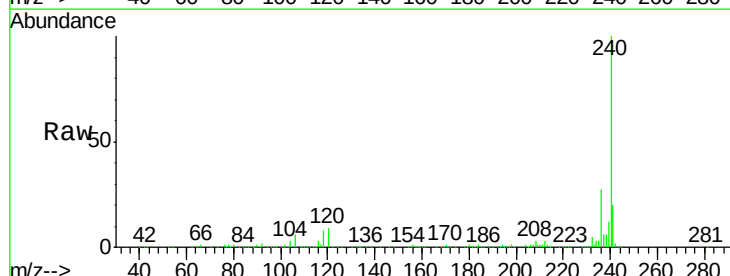

Abundance Ion 240.00 (239.70 to 240.70): E
Ion 120.00 (119.70 to 120.70): E
Ion 236.00 (235.70 to 236.70): E

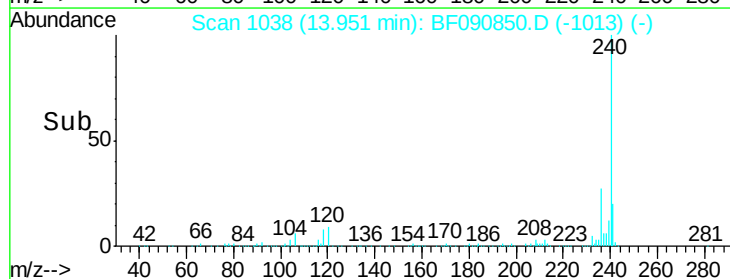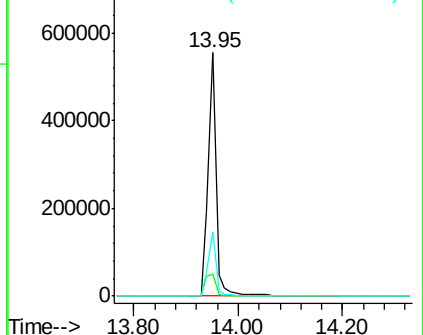

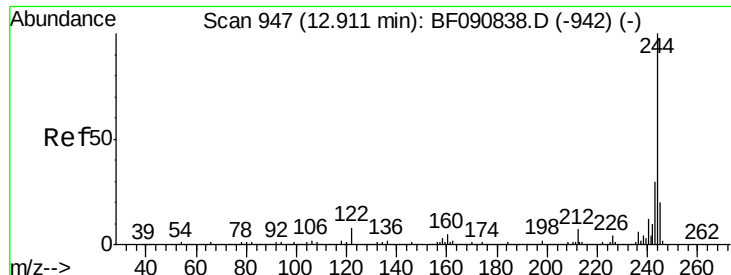

#78

Terphenyl-d14

Concen: 85.29 ng

RT: 12.90 min Scan# 946

Delta R.T. -0.02 min

Lab File: BF090850.D

Acq: 26 Oct 2016 19:55

Instrument :


BNA_F

ClientSampleId :

PB94315TB

Tot Ion:244 Resp: 2009693




Ion	Ratio	Lower	Upper
244	100		
212	7.3	4.3	6.5#
122	13.6	17.4	26.2#

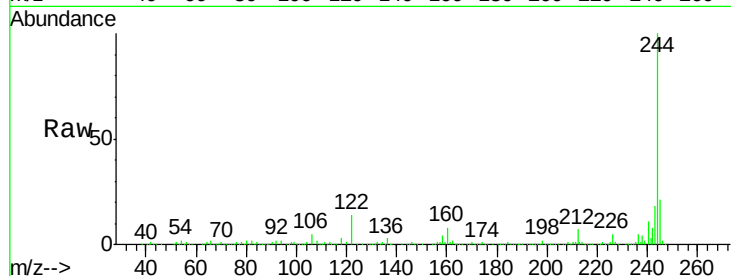

Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

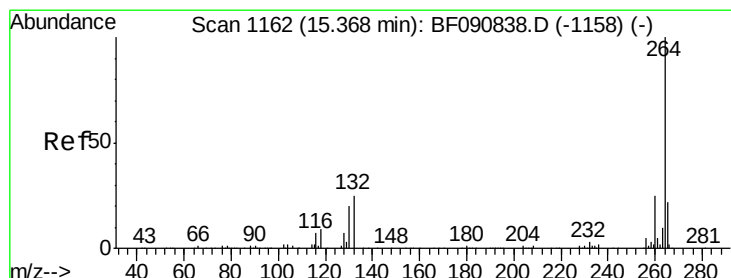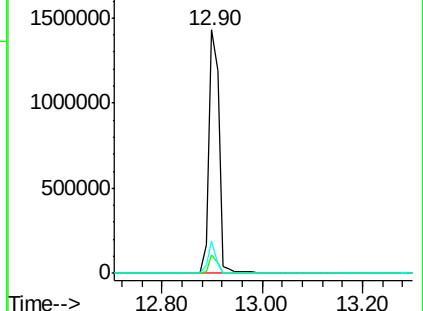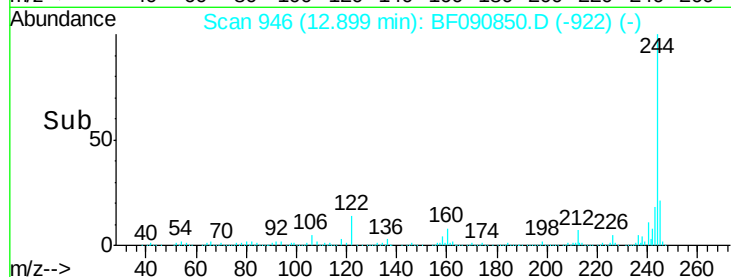

#86

Perylene-d12

Concen: 20.00 ng

RT: 15.37 min Scan# 1162


Delta R.T. -0.01 min

Lab File: BF090850.D

Acq: 26 Oct 2016 19:55

Tgt Ion:264 Resp: 448841

Ion	Ratio	Lower	Upper
264	100		
260	23.7	16.7	25.1
265	21.2	17.2	25.8

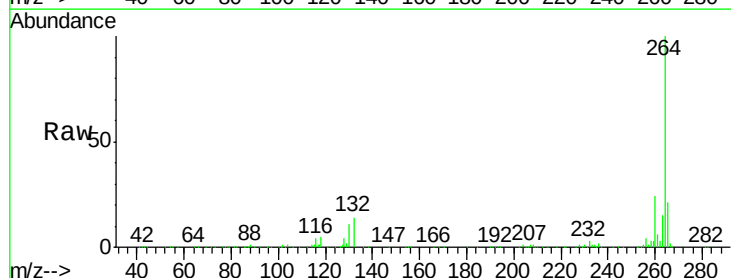

Abundance Ion 264.00 (263.70 to 264.70): E

Ion 260.00 (259.70 to 260.70): E

Ion 265.00 (264.70 to 265.70): E

