


Data Path : Z:\HPCHEM1\BNA_F\DATA\BF102616\
 Data File : BF090833.D
 Acq On : 26 Oct 2016 10:45
 Operator : UM/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF102616.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Oct 26 16:35:31 2016

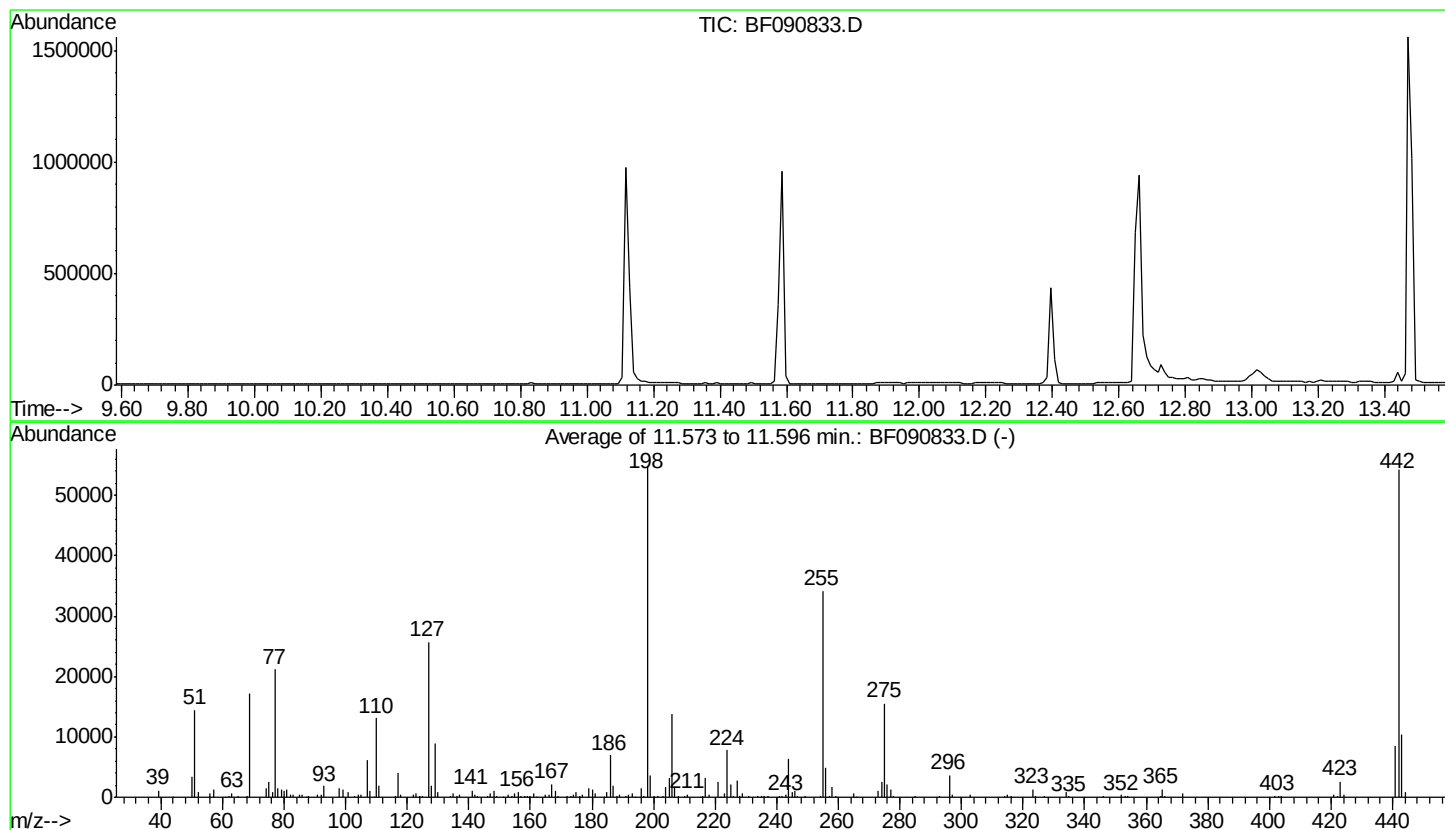

AutoFind: Scans 830, 831, 832; Background Corrected with Scan 826

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	26.4	14511	PASS
68	69	0.00	2	1.8	308	PASS
69	198	0.00	100	31.4	17218	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	46.7	25661	PASS
197	198	0.00	2	0.3	139	PASS
198	198	100	100	100.0	54912	PASS
199	198	5	9	6.5	3587	PASS
275	198	10	60	28.4	15573	PASS
365	198	1	100	2.4	1318	PASS
441	442	0.01	24	15.7	8486	PASS
442	198	50	100	98.6	54170	PASS
443	442	15	24	19.3	10432	PASS