


Data Path : Z:\HPCHEM1\BNA F\DATA\BF102616\
Data File : BF090843.D
Acq On : 26 Oct 2016 15:46
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF102616.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Wed Oct 26 16:35:31 2016

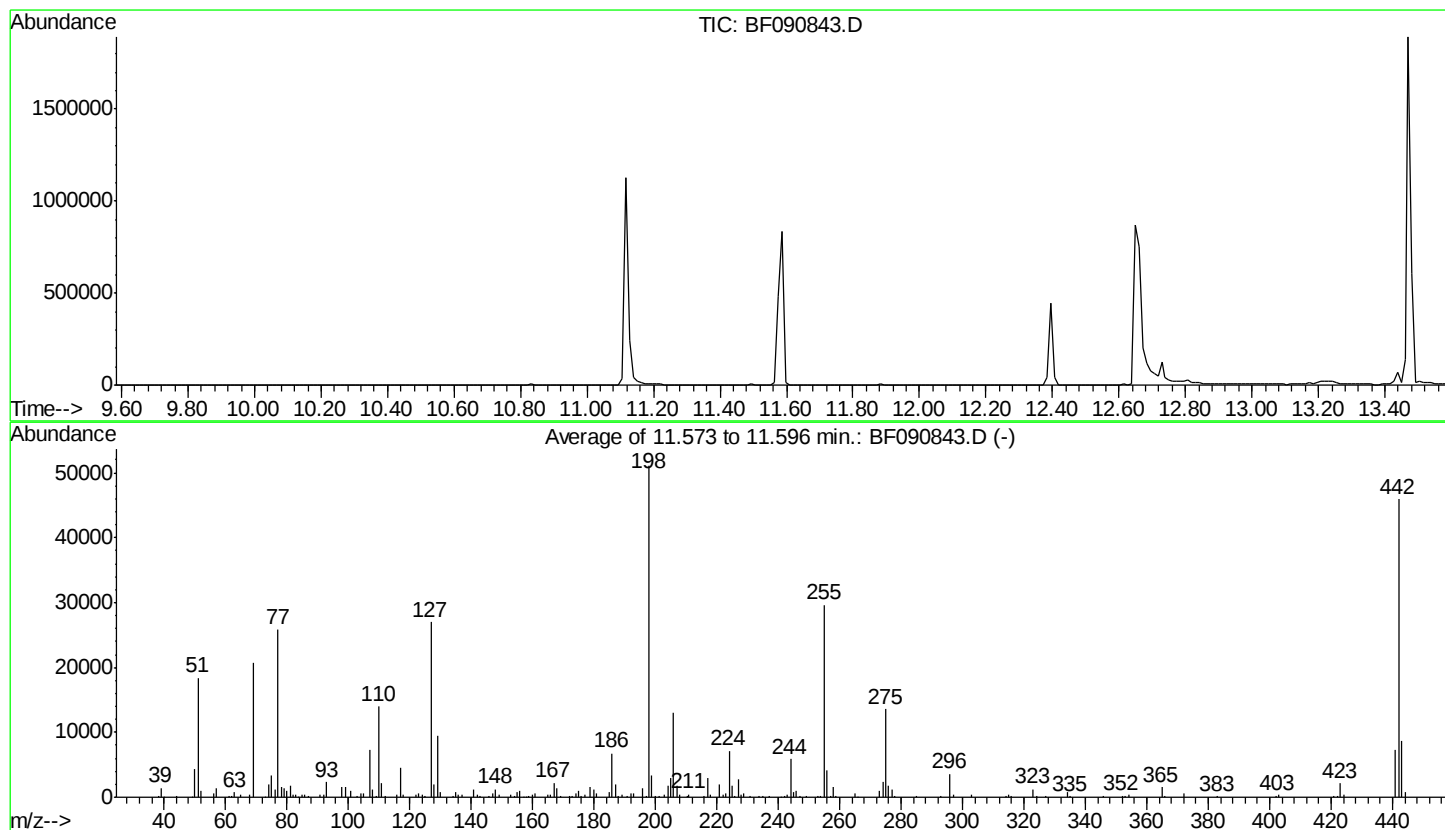

AutoFind: Scans 830, 831, 832; Background Corrected with Scan 826

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	35.9	18363	PASS
68	69	0.00	2	1.6	340	PASS
69	198	0.00	100	40.6	20776	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	52.7	26946	PASS
197	198	0.00	2	0.3	130	PASS
198	198	100	100	100.0	51112	PASS
199	198	5	9	6.6	3365	PASS
275	198	10	60	26.6	13591	PASS
365	198	1	100	2.9	1495	PASS
441	442	0.01	24	16.1	7382	PASS
442	198	50	100	89.8	45904	PASS
443	442	15	24	19.1	8769	PASS