
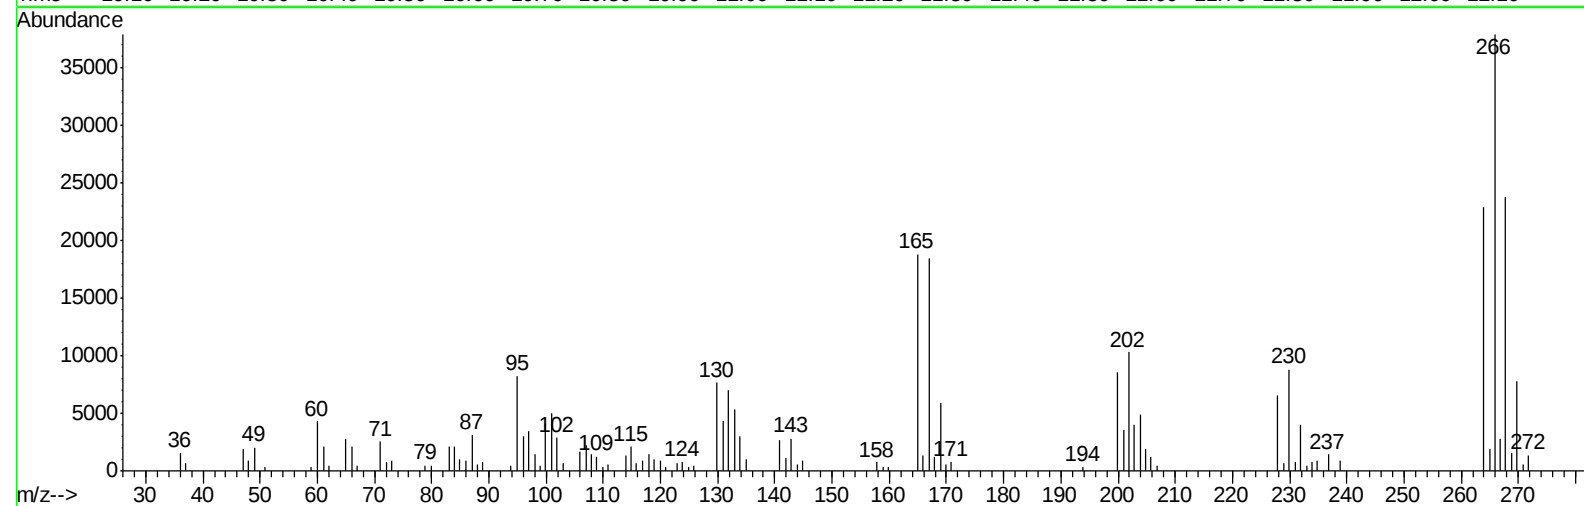


Data Path : Z:\HPCHEM1\BNA F\DATA\BF102617\  
Data File : BF099855.D  
Acq On : 26 Oct 2017 11:48  
Operator : SJ/JU  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 27 02:02:49 2017  
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF102317.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Thu Oct 26 16:31:52 2017  
Response via : Initial Calibration

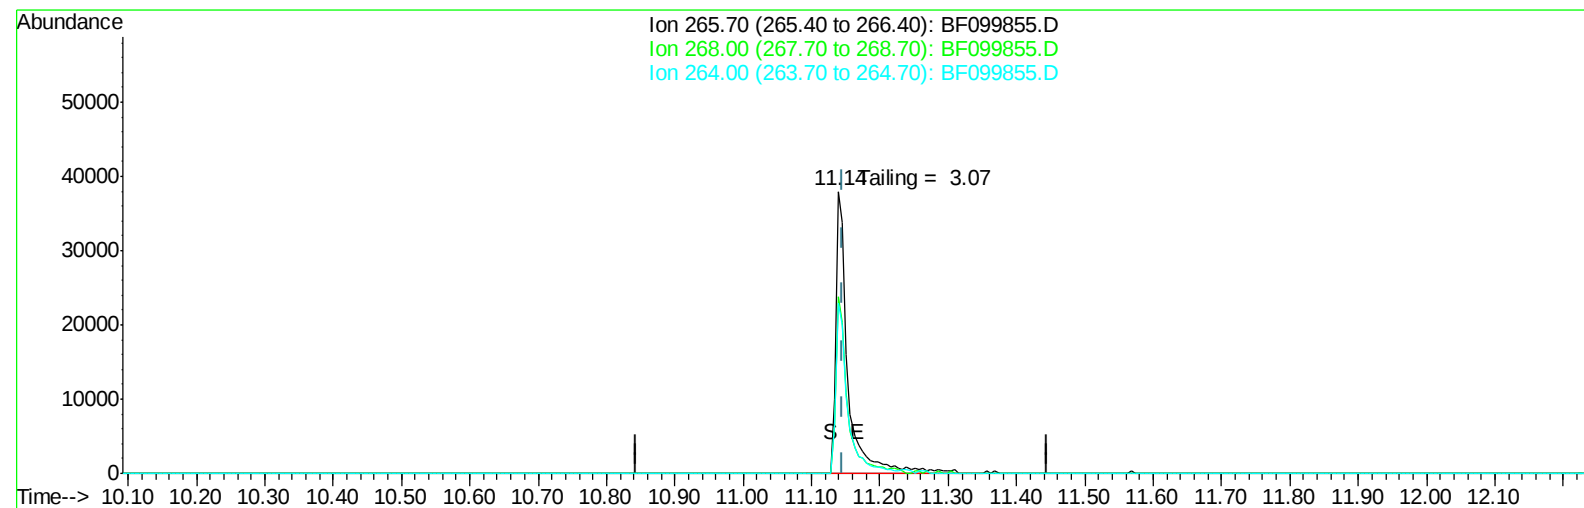

TIC: BF099855.D

(69) Pentachlorophenol (C)



11.139min (-0.006) 74956.81ng

response 45880

| Ion    | Exp%  | Act%  |
|--------|-------|-------|
| 265.70 | 100   | 100   |
| 268.00 | 63.90 | 62.63 |
| 264.00 | 61.90 | 60.48 |
| 0.00   | 0.00  | 0.00  |

Data Path : Z:\HPCHEM1\BNA F\DATA\BF102617\  
Data File : BF099855.D  
Acq On : 26 Oct 2017 11:48  
Operator : SJ/JU  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 27 02:02:49 2017  
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF102317.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Thu Oct 26 16:31:52 2017  
Response via : Initial Calibration

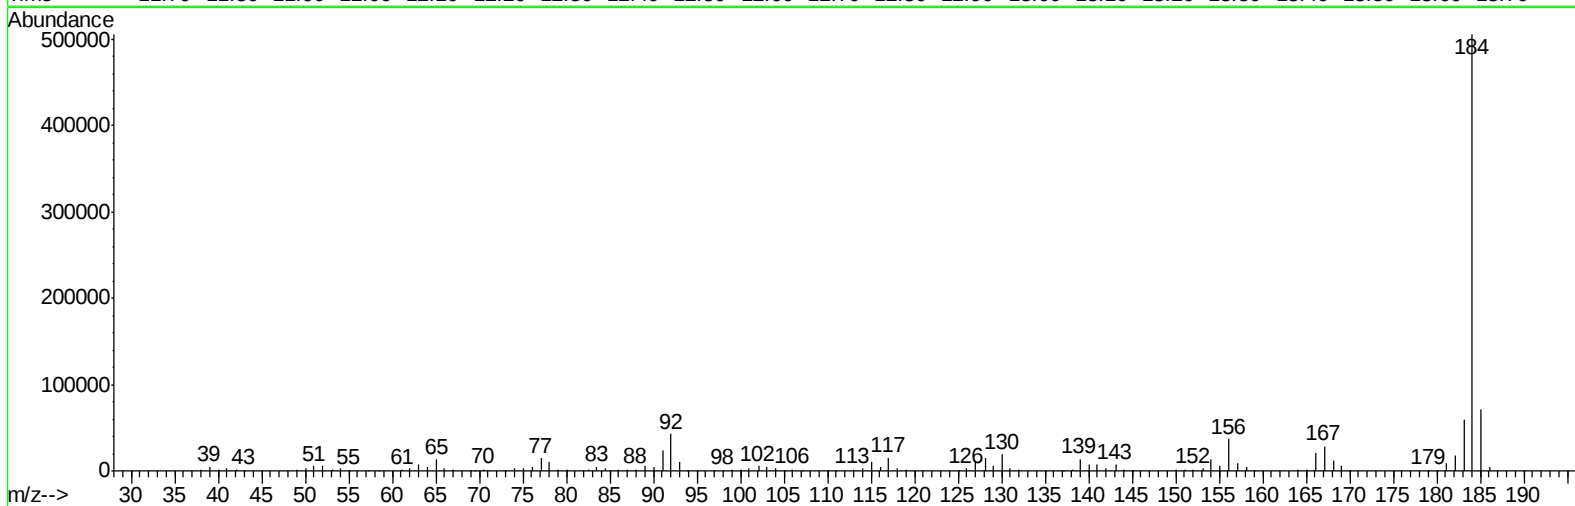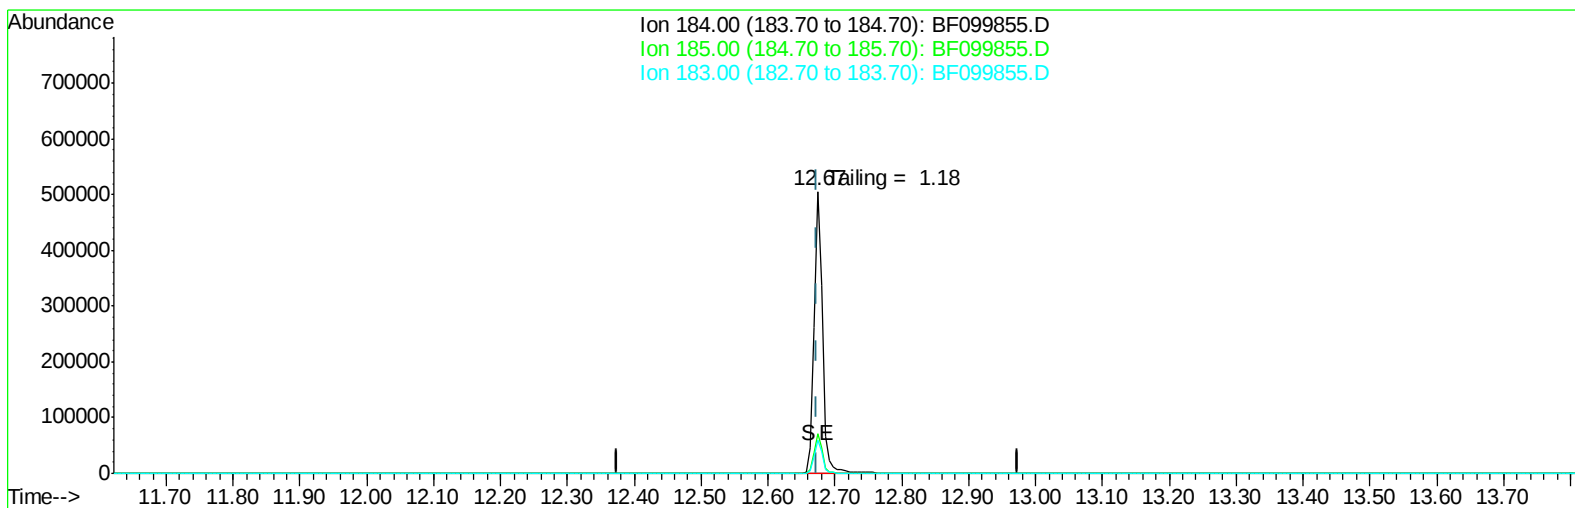

TIC: BF099855.D

(76) Benzidine

12.674min (+0.000) 0.00ng

response 456308

| Ion    | Exp%  | Act%  |
|--------|-------|-------|
| 184.00 | 100   | 100   |
| 185.00 | 15.70 | 13.94 |
| 183.00 | 11.60 | 11.74 |
| 0.00   | 0.00  | 0.00  |