

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF102617\
 Data File : BF099863.D
 Acq On : 26 Oct 2017 16:02
 Operator : SJ/JU
 Sample : I6089-01 5X
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 SB-01

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF102317.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	4.992	492	494	503	rBV	20225	31108	5.76%	0.626%
2	5.416	563	566	587	rBV	150334	224837	41.64%	4.525%
3	6.439	737	740	754	rBV	177479	246621	45.68%	4.963%
4	6.569	759	762	770	rVB	291131	279870	51.83%	5.632%
5	6.792	797	800	811	rBV	400431	332207	61.53%	6.686%
6	6.945	824	826	835	rBV	210885	207075	38.35%	4.167%
7	7.363	894	897	912	rBV	142375	146494	27.13%	2.948%
8	8.075	1015	1018	1026	rBV	534067	468990	86.86%	9.438%
9	8.645	1110	1115	1119	rVB	7107	8331	1.54%	0.168%
10	9.151	1198	1201	1210	rBV	400291	329914	61.10%	6.639%
11	9.839	1314	1318	1325	rBV	597124	534115	98.92%	10.749%
12	10.551	1436	1439	1442	rBV	33229	29420	5.45%	0.592%
13	10.633	1450	1453	1463	rBV	192551	175115	32.43%	3.524%
14	10.739	1467	1471	1479	rBV3	9256	15017	2.78%	0.302%
15	11.210	1548	1551	1556	rVB5	10355	12236	2.27%	0.246%
16	11.333	1568	1572	1581	rBV	576528	528291	97.84%	10.632%
17	11.551	1603	1609	1613	rBV7	6011	11899	2.20%	0.239%
18	11.851	1657	1660	1667	rBV5	12917	22622	4.19%	0.455%
19	12.639	1791	1794	1799	rBV6	15374	26690	4.94%	0.537%
20	12.915	1838	1841	1848	rVB	366349	322581	59.74%	6.492%
21	13.986	2020	2023	2027	rBV	521959	475643	88.09%	9.572%
22	15.462	2270	2274	2283	rVB	382342	539932	100.00%	10.866%


Sum of corrected areas: 4969008

Data Path : Z:\HPCHEM1\BNA F\DATA\BF102617\
Data File : BF099863.D
Acq On : 26 Oct 2017 16:02
Operator : SJ/JU
Sample : I6089-01 5X
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
SB-01

Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF102317.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

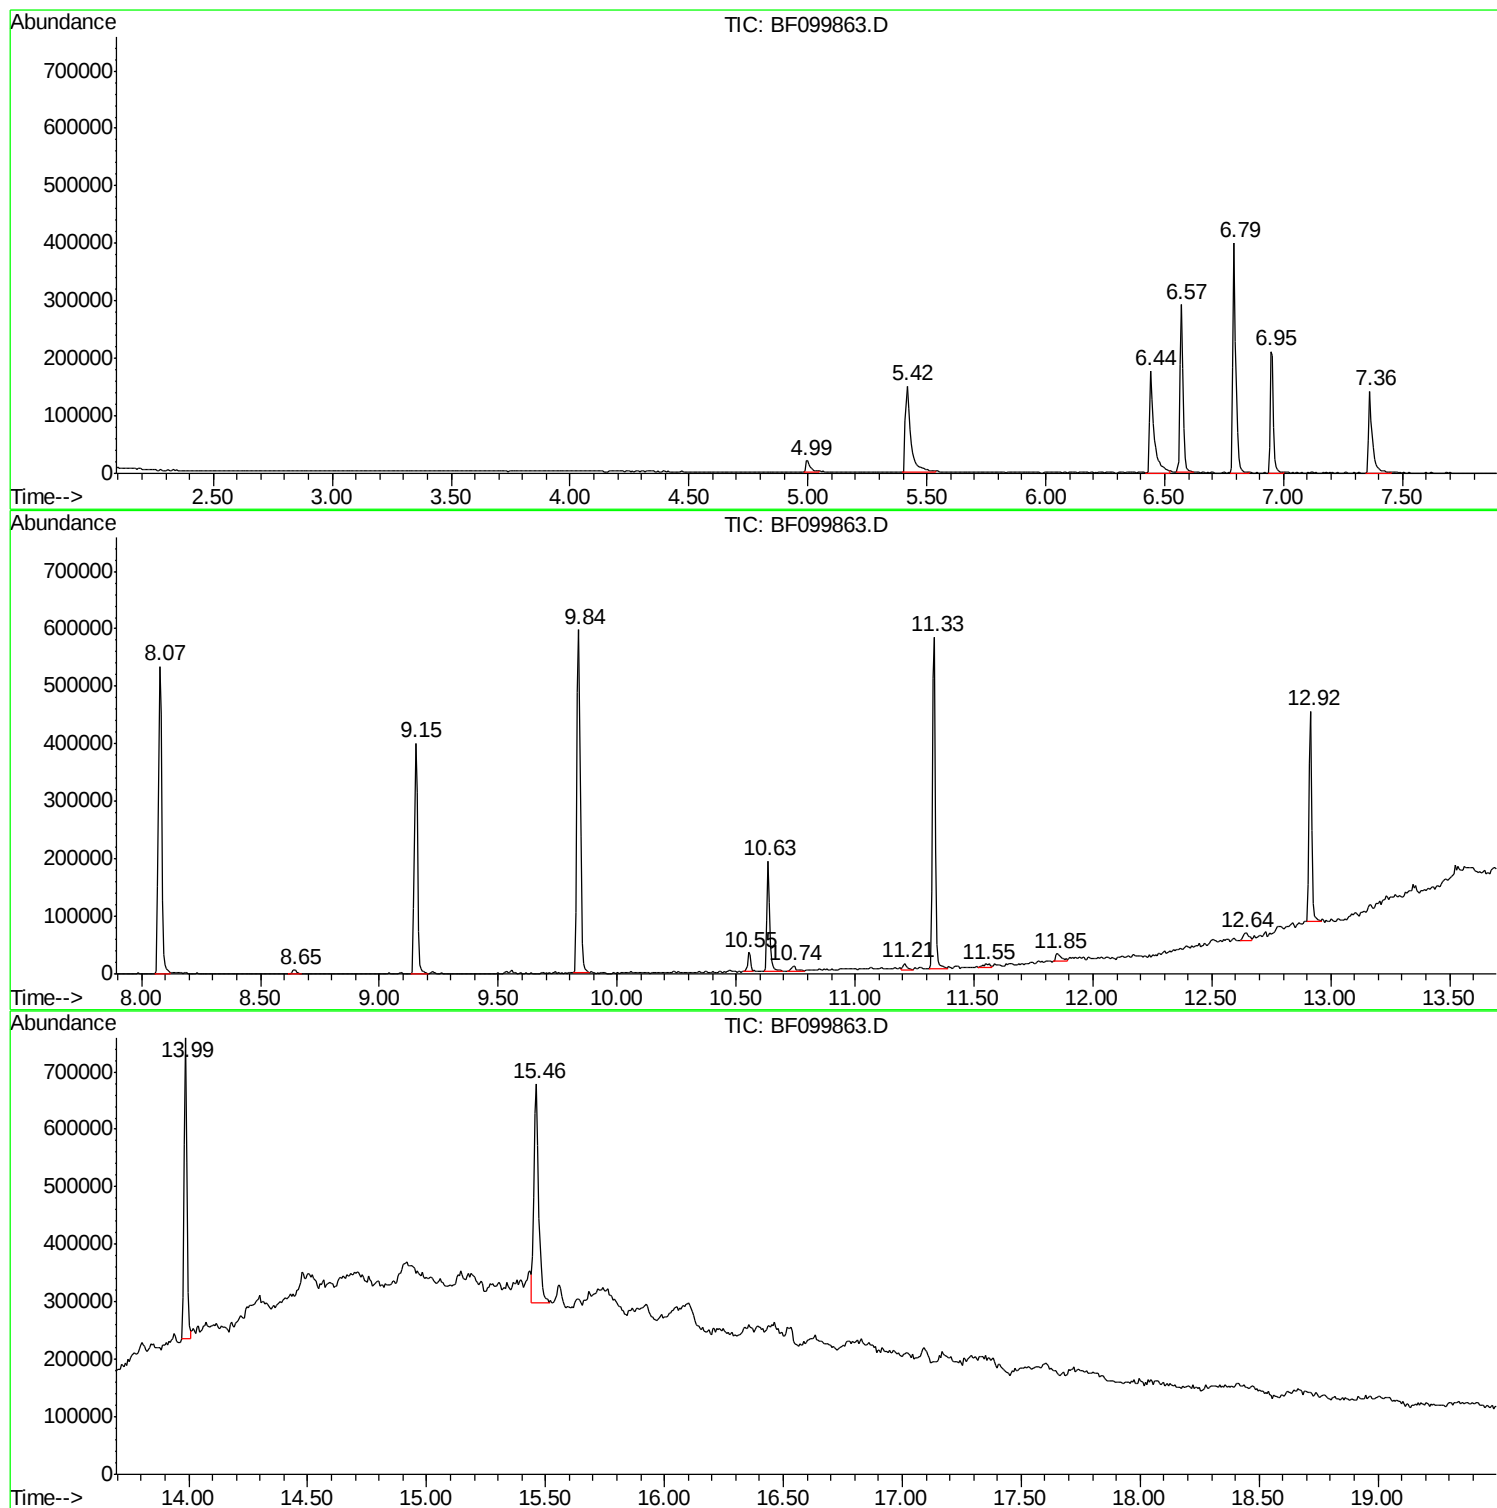

Data Path : Z:\HPCHEM1\BNA F\DATA\BF102617\
Data File : BF099863.D
Acq On : 26 Oct 2017 16:02
Operator : SJ/JU
Sample : I6089-01 5X
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
SB-01










Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF102317.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 unknown6.57 Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
6.57	16.85 ng	279870	1,4-Dichlorobenzene-d4	6.79

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	3-Chloro-6-fluoro-pyrazine	132	C4H2ClFN2	1000146-10-7	38
2		(E)-3-Chloro-2-methyl-2-pentenal	132	C6H9ClO	031357-76-3	25
3		1H-Indazole, 7-methyl-	132	C8H8N2	1000316-00-7	10
4		4-Chloro-6-fluoro-pyrimidine	132	C4H2ClFN2	051422-01-6	9
5		1-Aminoindan	133	C9H11N	034698-41-4	9

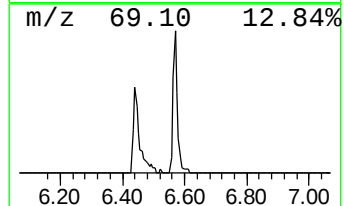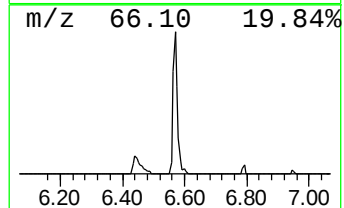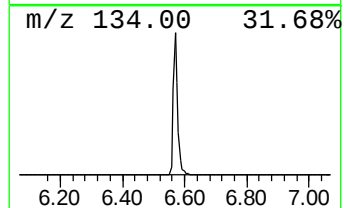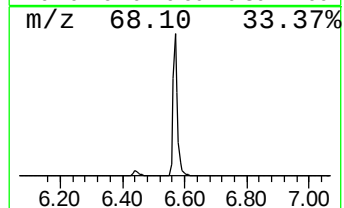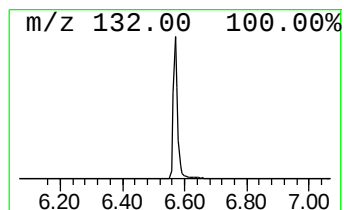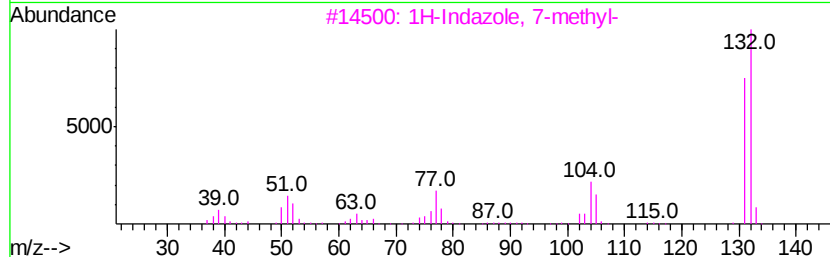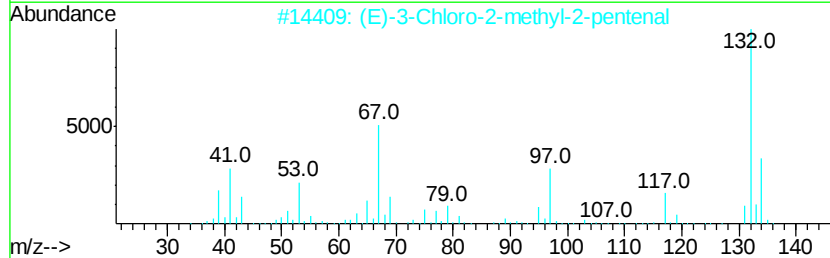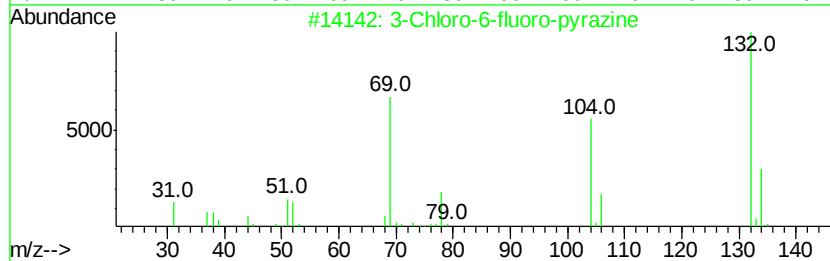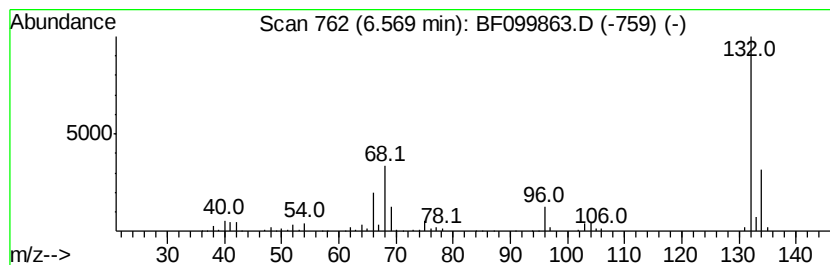

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF102617\
Data File : BF099863.D
Acq On : 26 Oct 2017 16:02
Operator : SJ/JU
Sample : I6089-01 5X
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
SB-01

Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF102317.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
unknown6.57	6.57	16.9	ng	279870	1	6.79	332207	20.0